

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022522\
 Data File : BF127067.D
 Acq On : 25 Feb 2022 13:17
 Operator : CG\JU
 Sample : PB142924BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142924BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	547	552	555	rBV	2847767	2569553	65.55%	12.410%
2	6.534	716	722	725	rBV	2614008	2650273	67.61%	12.800%
3	6.904	781	785	788	rBV	629768	516044	13.16%	2.492%
4	7.469	875	881	884	rBV	1841281	1835722	46.83%	8.866%
5	8.187	998	1003	1006	rBV	801964	694430	17.72%	3.354%
6	9.263	1180	1186	1189	rBV	3575000	3316963	84.62%	16.019%
7	9.945	1297	1302	1305	rBV	965585	779746	19.89%	3.766%
8	10.739	1432	1437	1440	rBV	2687348	2335796	59.59%	11.281%
9	11.439	1552	1556	1559	rBV	945348	835850	21.32%	4.037%
10	13.027	1821	1826	1829	rBV	4027674	3919826	100.00%	18.931%
11	14.086	2002	2006	2009	rBV	827598	706354	18.02%	3.411%
12	15.586	2256	2261	2268	rVB2	433484	545439	13.91%	2.634%




Sum of corrected areas: 20705996

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022522\
Data File : BF127067.D
Acq On : 25 Feb 2022 13:17
Operator : CG\JU
Sample : PB142924BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142924BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

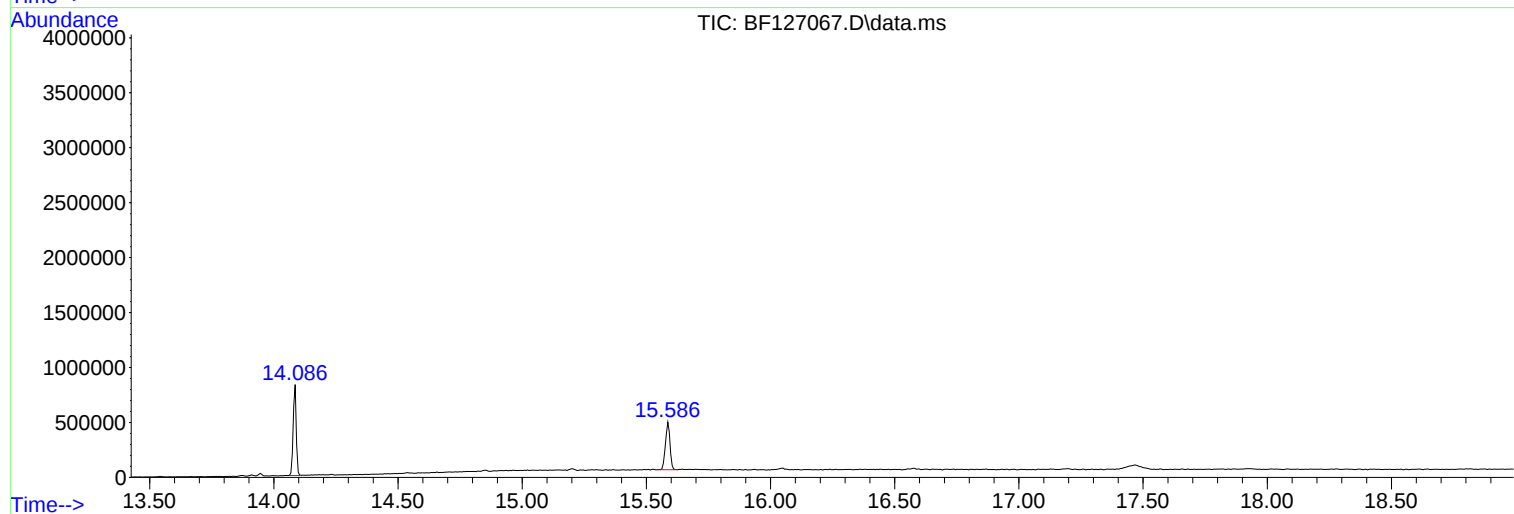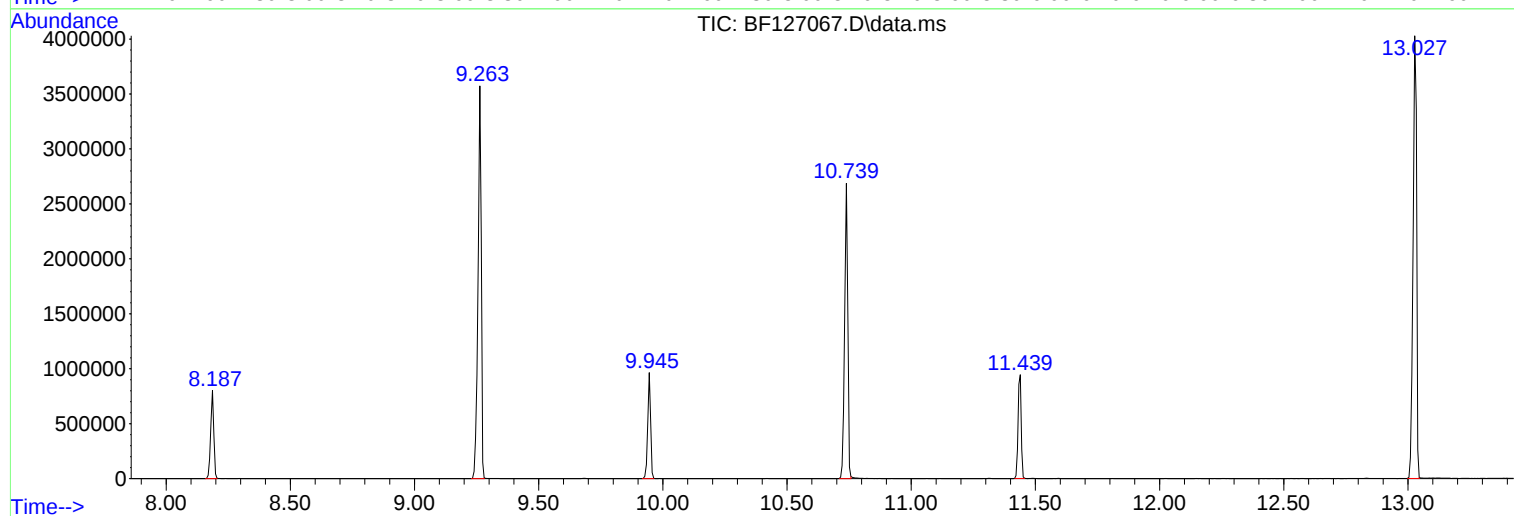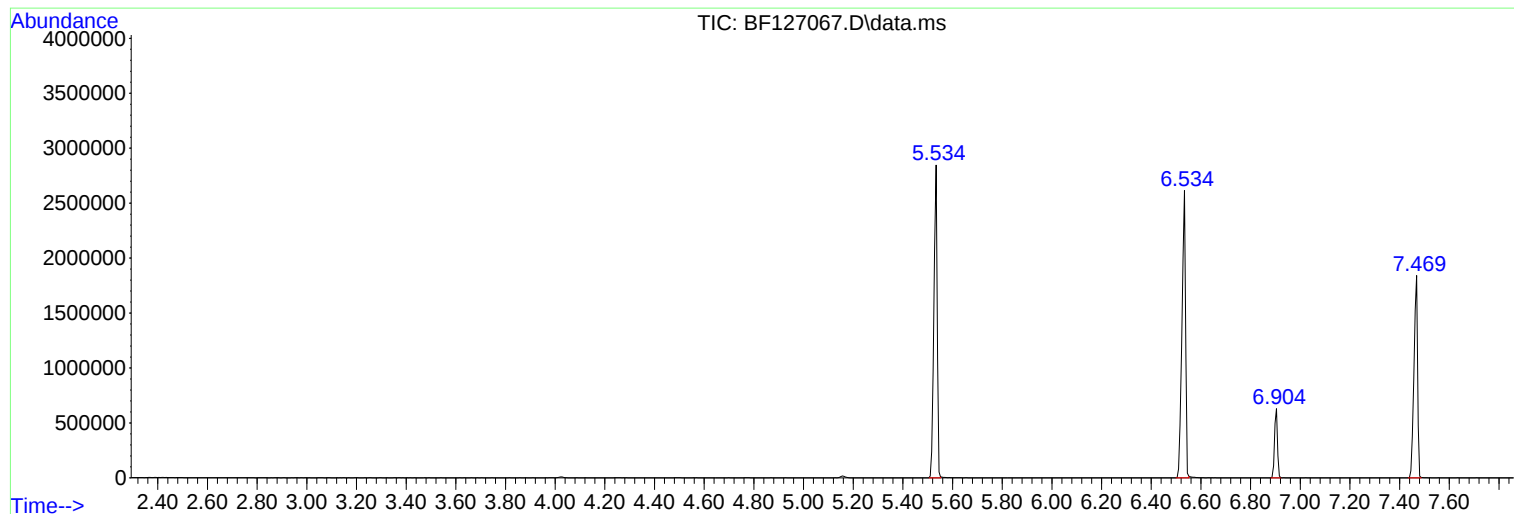

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022522\
Data File : BF127067.D
Acq On : 25 Feb 2022 13:17
Operator : CG\JU
Sample : PB142924BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142924BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022522\
Data File : BF127067.D
Acq On : 25 Feb 2022 13:17
Operator : CG\JU
Sample : PB142924BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142924BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------