
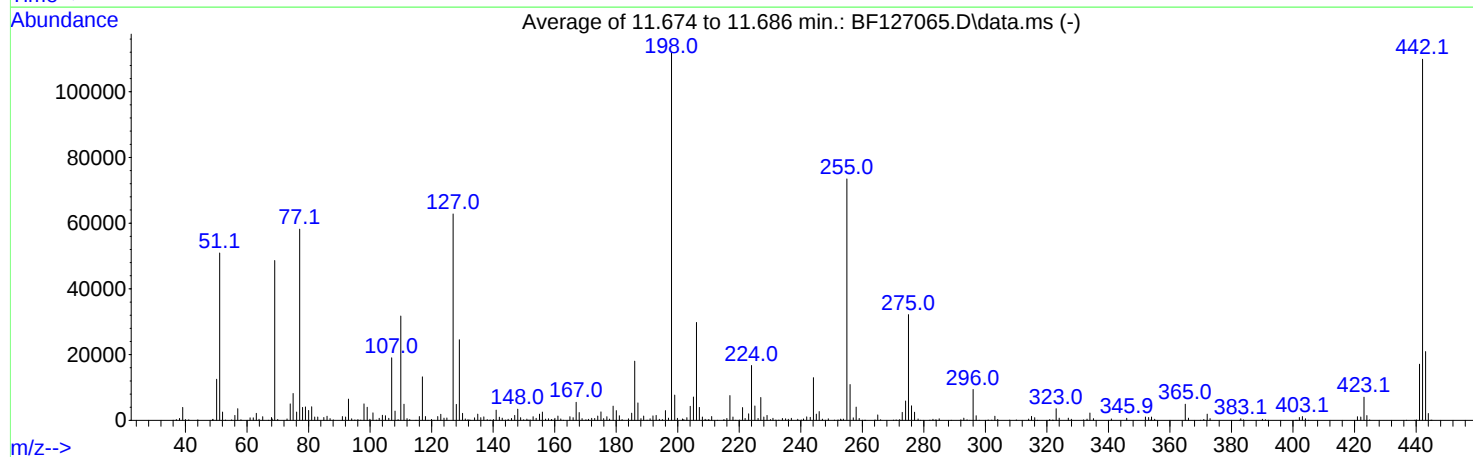


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022522\
 Data File : BF127065.D
 Acq On : 25 Feb 2022 11:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 24 02:10:57 2022

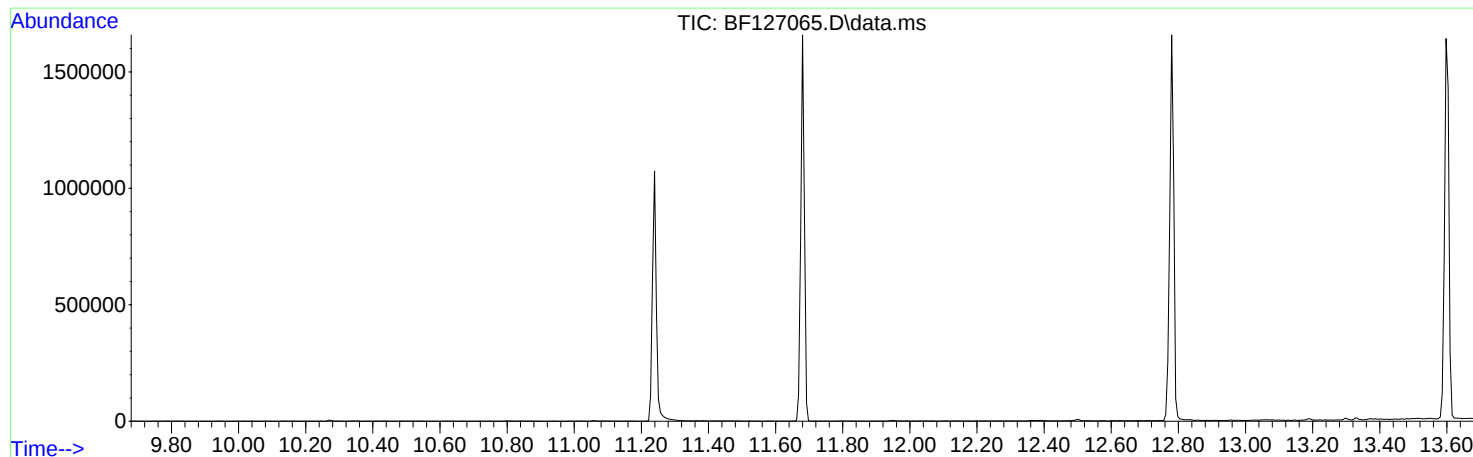




AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	50923	PASS
68	69	0.00	2	1.8	895	PASS
69	198	0.00	100	43.5	48648	PASS
70	69	0.00	2	0.6	297	PASS
127	198	10	80	56.1	62779	PASS
197	198	0.00	2	0.6	675	PASS
198	198	100	100	100.0	111920	PASS
199	198	5	9	6.9	7691	PASS
275	198	10	60	28.8	32187	PASS
365	198	1	100	4.4	4939	PASS
441	198	0.01	100	15.3	17110	PASS
442	198	50	100	98.2	109893	PASS
443	442	15	24	19.0	20913	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022522\
Data File : BF127065.D
Acq On : 25 Feb 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 26 05:25:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 24 02:10:57 2022
Response via : Initial Calibration

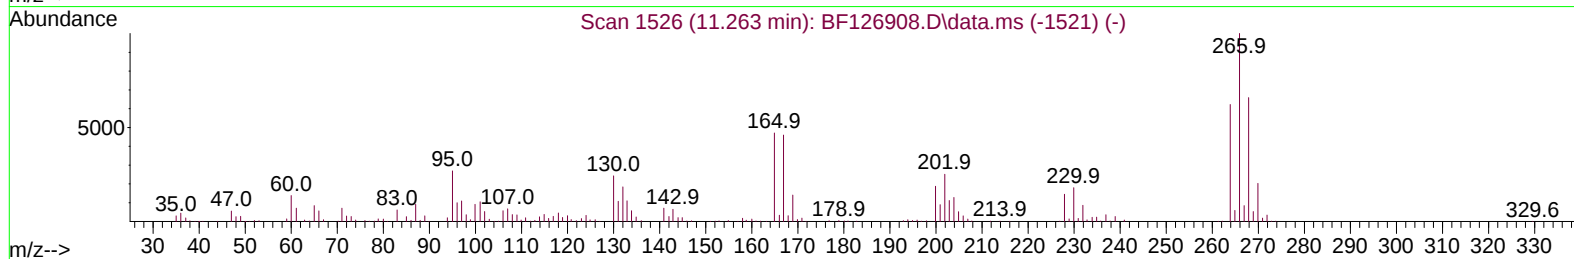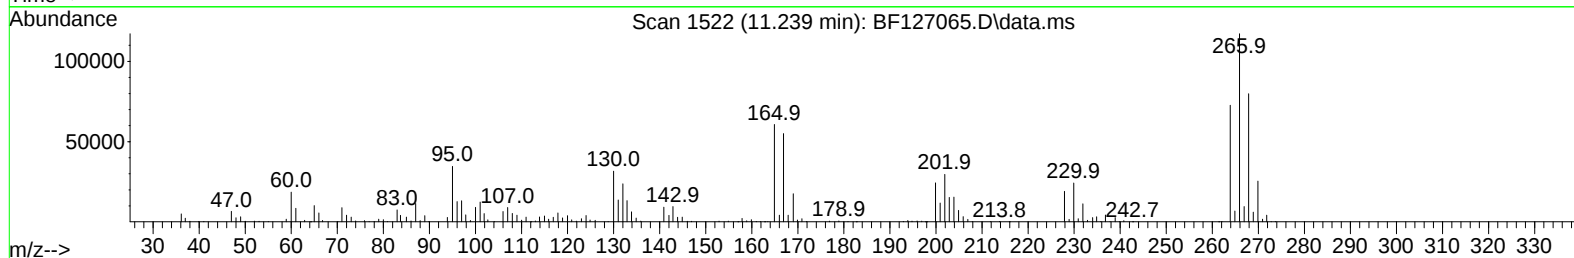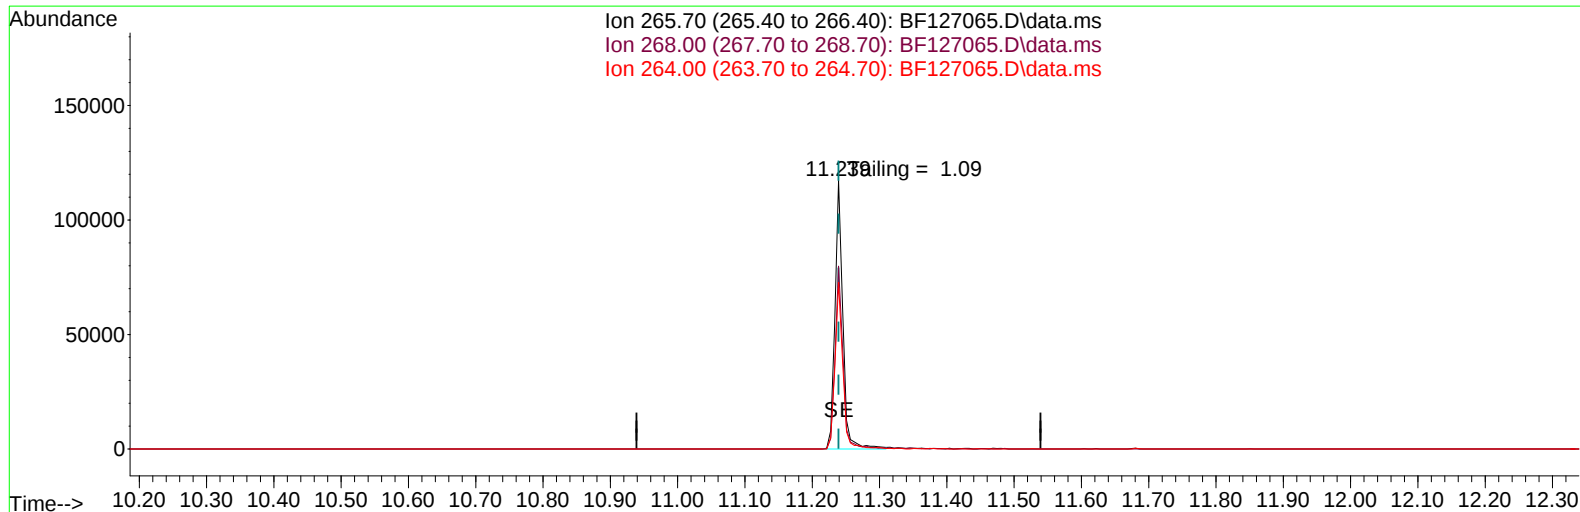

TIC: BF127065.D\data.ms

(70) Pentachlorophenol (C)

11.239min (0.000) 24575.57 ng




response 96172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	68.13
264.00	63.00	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022522\
 Data File : BF127065.D
 Acq On : 25 Feb 2022 11:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 26 05:25:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 24 02:10:57 2022
 Response via : Initial Calibration

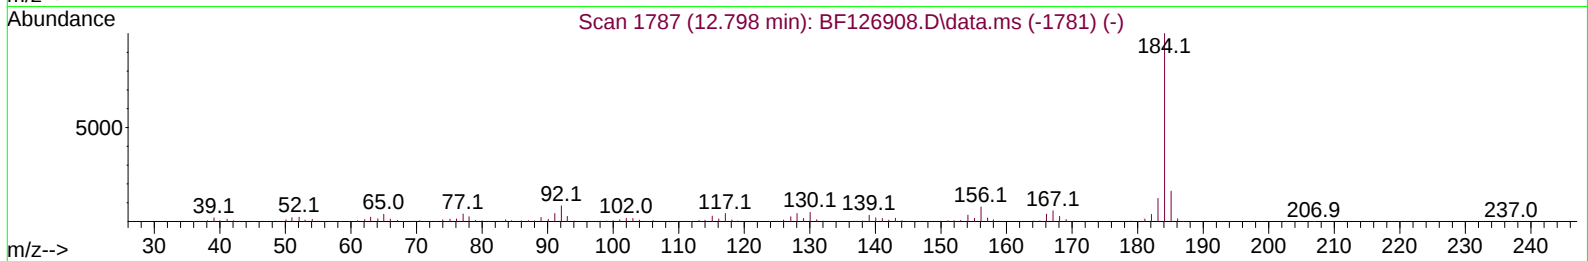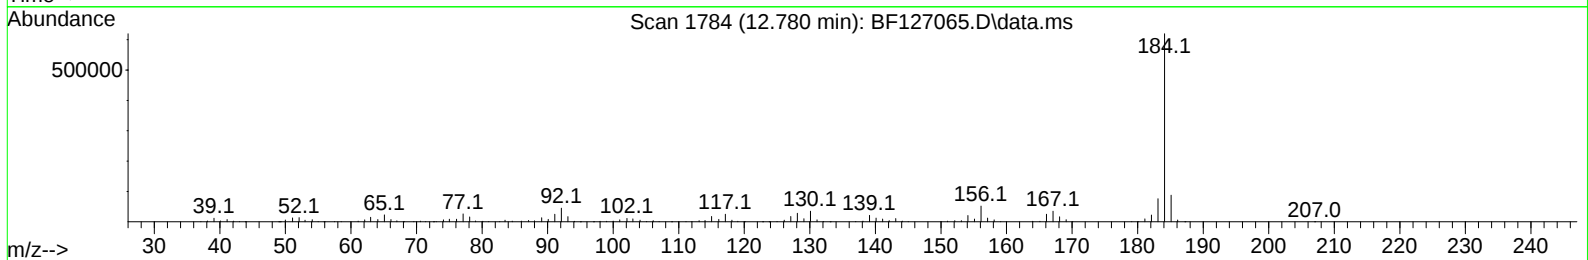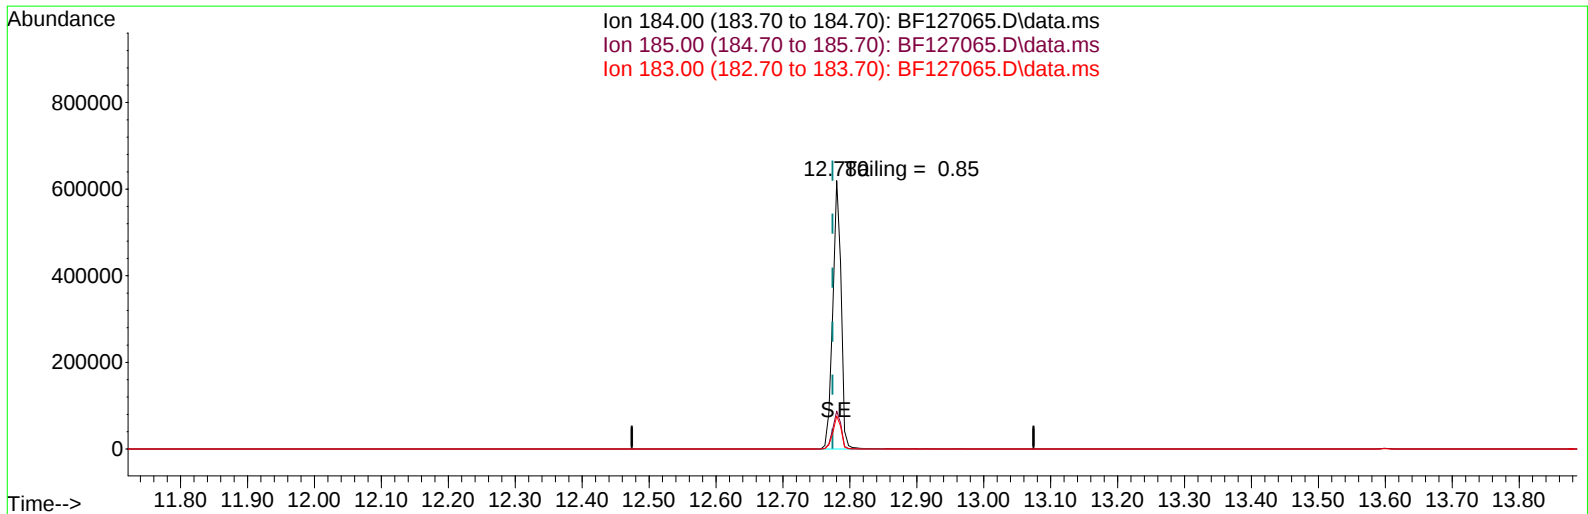

TIC: BF127065.D\data.ms

(77) Benzidine

12.780min (+ 0.006) 0.00 ng

response 538173

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.17
183.00	10.20	12.31#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/25/2022	BNA_F	<u>BF127065.D</u>
Compound Name	Response	Retention Time
DDT	259761	13.598
DDD	2733	13.298
DDE	380	12.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3113	262874	1.18

Instrument :
BNA_F
ClientSampleId :
DFTPP