
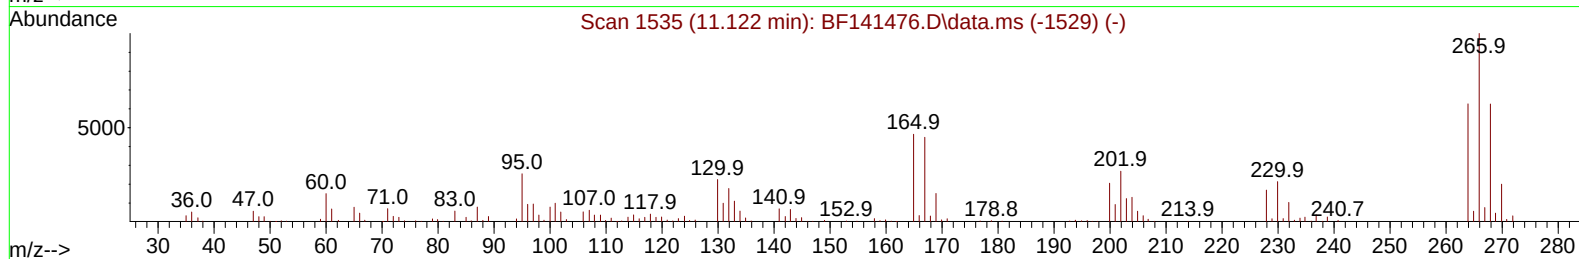
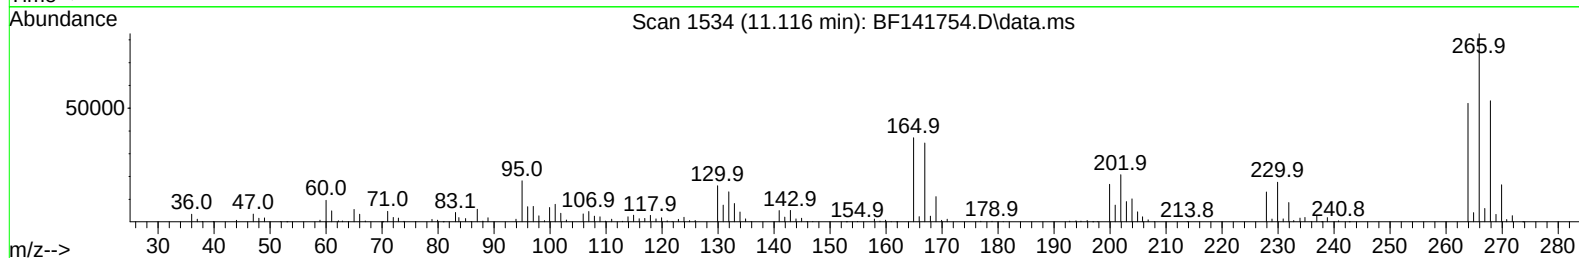


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022525\
Data File : BF141754.D
Acq On : 25 Feb 2025 09:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 09:54:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

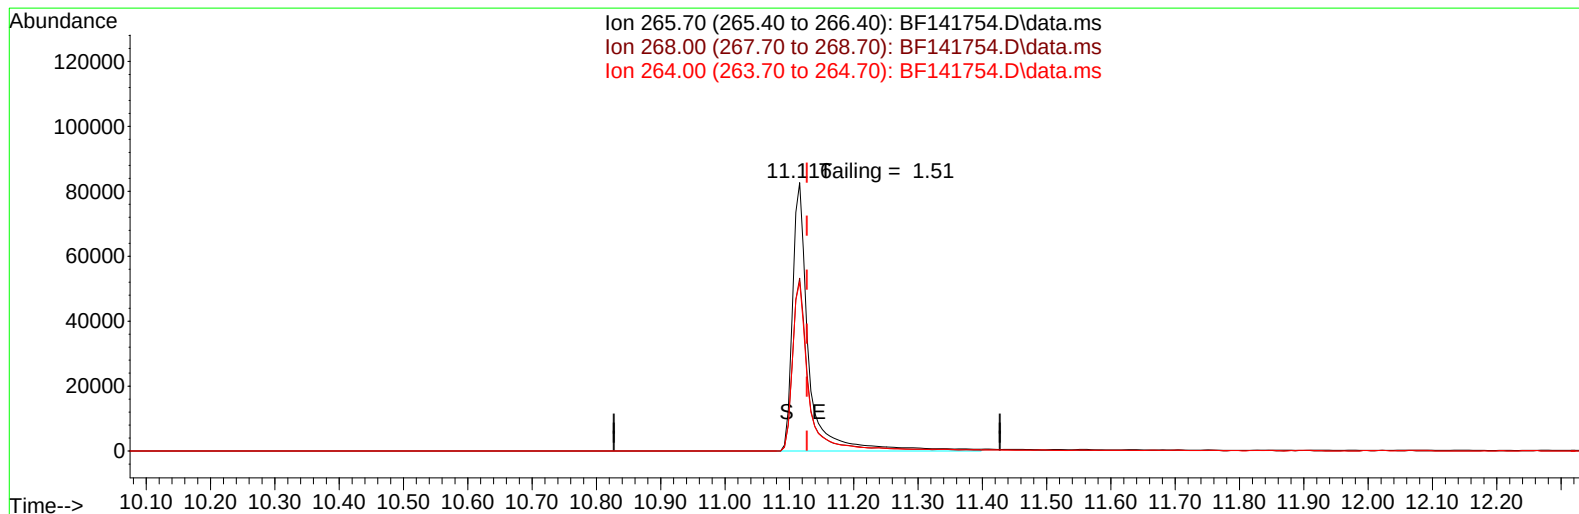

TIC: BF141754.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.011) 155220.49 ng

response 143922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.39
264.00	62.60	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022525\
Data File : BF141754.D
Acq On : 25 Feb 2025 09:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 09:54:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

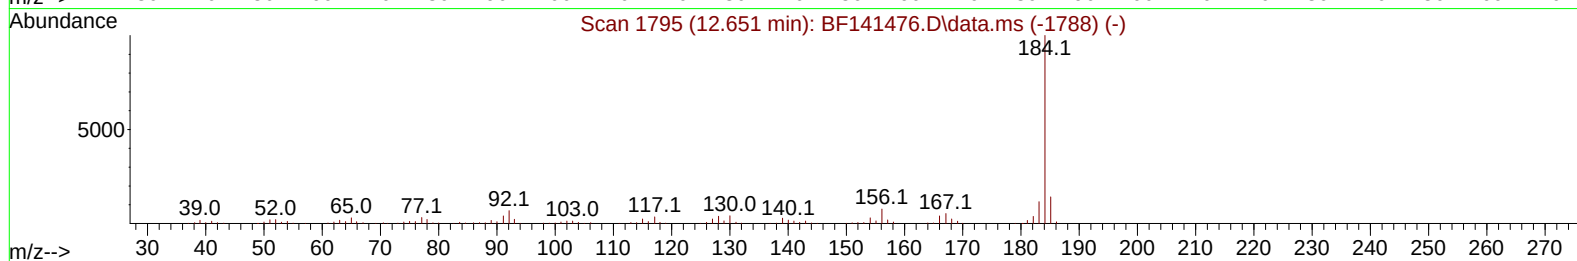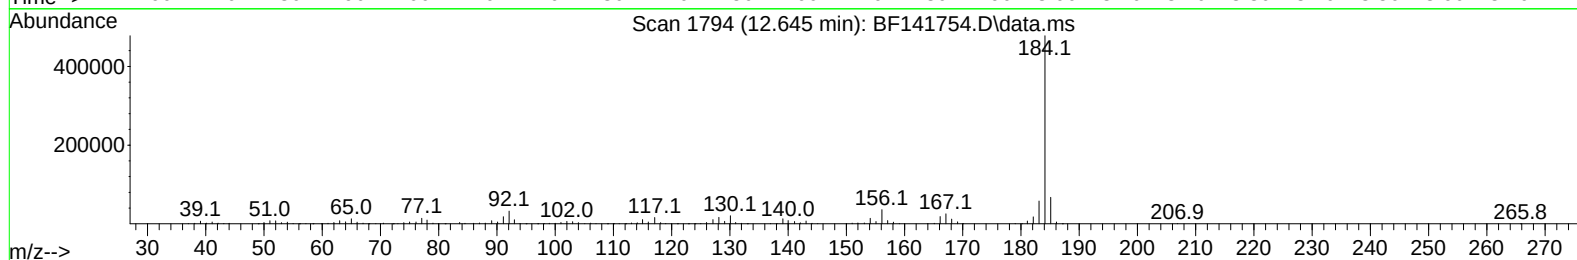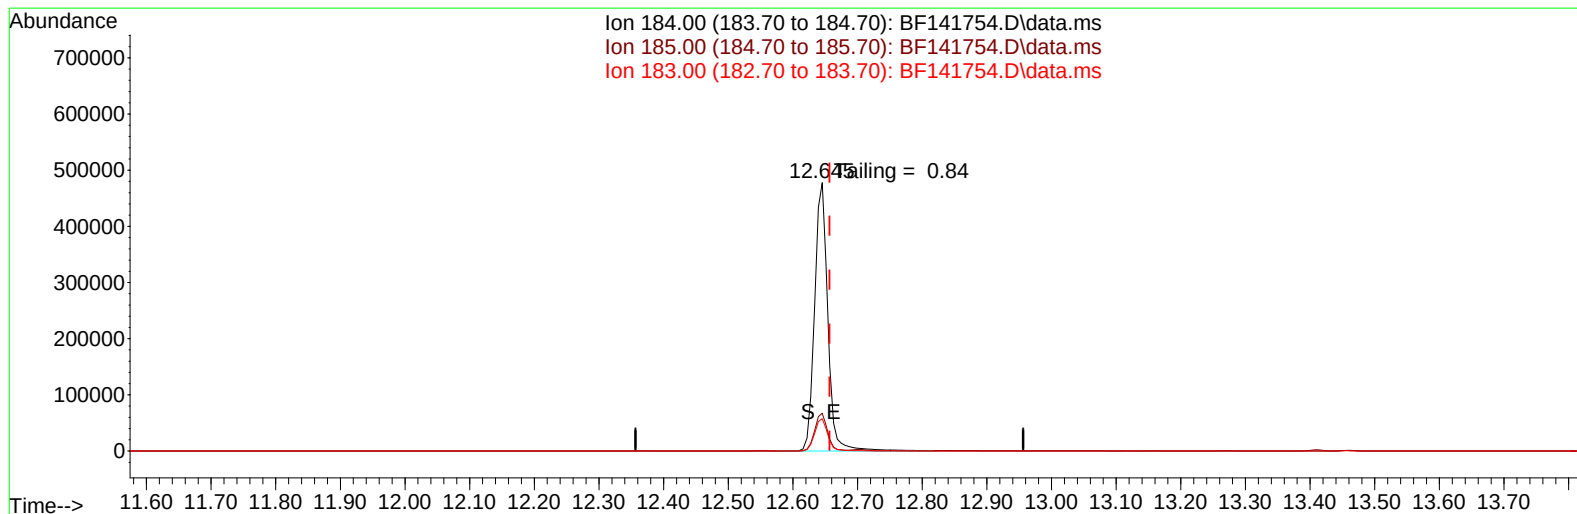

TIC: BF141754.D\data.ms

(77) Benzidine

12.645min (-0.012) 0.00 ng

response 681801

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	11.60	12.08
0.00	0.00	0.00