

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022525\
Data File : BF141756.D
Acq On : 25 Feb 2025 11:04
Operator : RC/JU
Sample : PB166840BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166840BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.410	559	564	595	rBV	1902786	2714925	80.19%	14.037%
2	6.428	731	737	757	rBV	1839584	2664479	78.70%	13.777%
3	6.781	792	797	810	rBV	396332	496715	14.67%	2.568%
4	7.345	887	893	934	rBV	1280293	1831568	54.10%	9.470%
5	8.063	1009	1015	1032	rBV	471040	676829	19.99%	3.500%
6	9.139	1192	1198	1213	rBV	2478183	3385488	100.00%	17.505%
7	9.816	1307	1313	1332	rBV	552380	772714	22.82%	3.995%
8	10.604	1442	1447	1474	rBV	1351598	1947711	57.53%	10.071%
9	11.298	1560	1565	1584	rBV	516879	761268	22.49%	3.936%
10	12.886	1829	1835	1840	rBV	2428111	3191607	94.27%	16.502%
11	13.939	2009	2014	2028	rBV	312329	478616	14.14%	2.475%
12	15.386	2254	2260	2274	rBV	229724	418659	12.37%	2.165%




Sum of corrected areas: 19340579

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022525\
Data File : BF141756.D
Acq On : 25 Feb 2025 11:04
Operator : RC/JU
Sample : PB166840BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166840BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

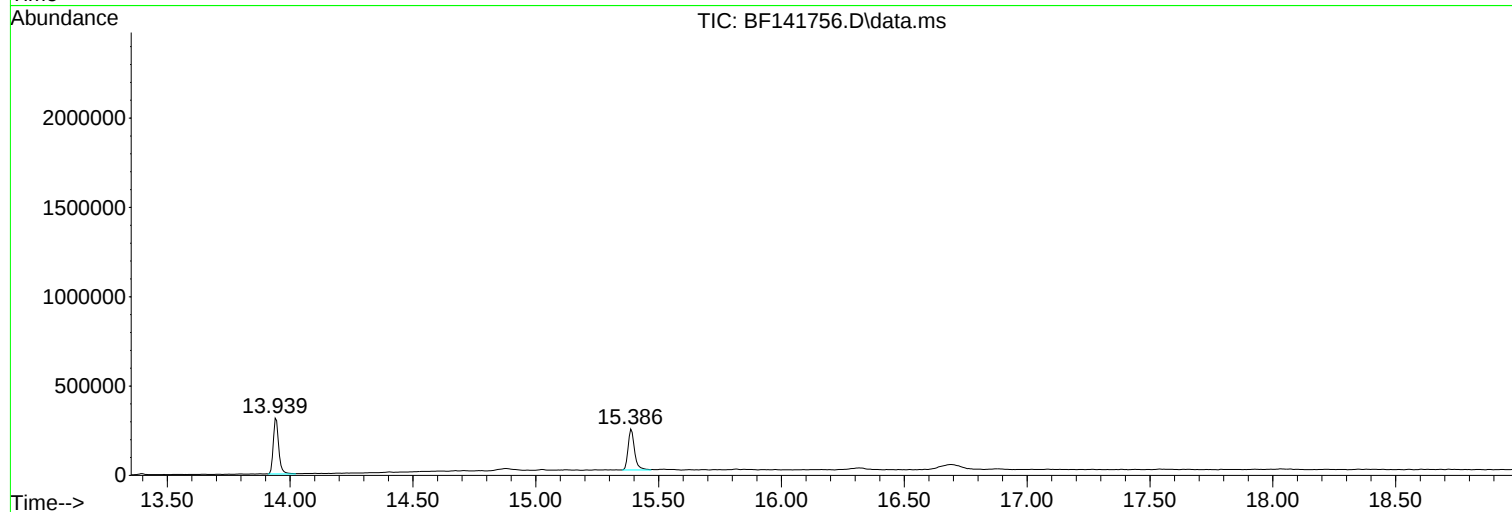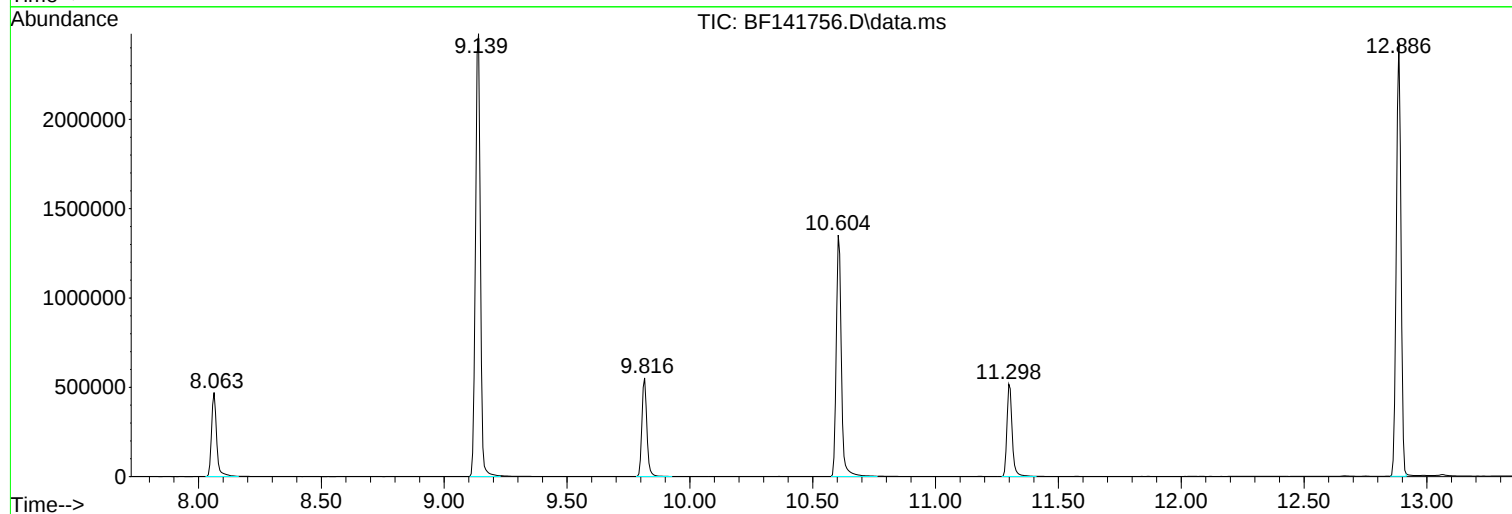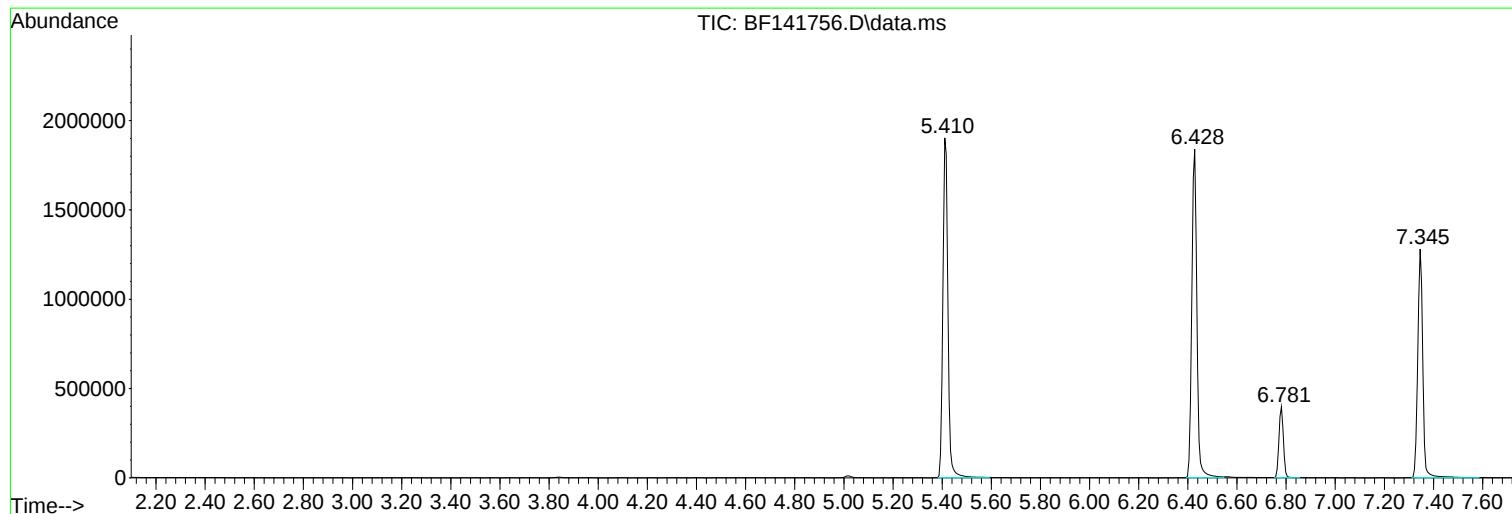

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022525\
Data File : BF141756.D
Acq On : 25 Feb 2025 11:04
Operator : RC/JU
Sample : PB166840BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166840BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022525\
Data File : BF141756.D
Acq On : 25 Feb 2025 11:04
Operator : RC/JU
Sample : PB166840BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166840BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------