
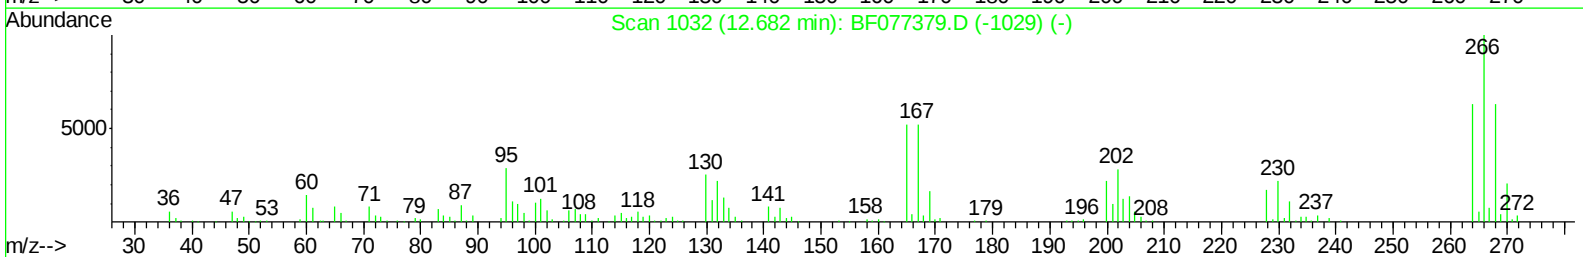
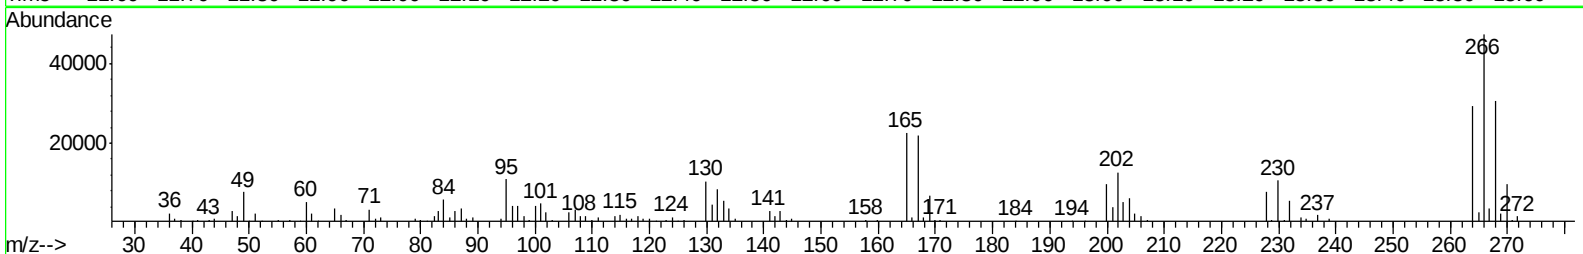


Data Path : Z:\HPCHEM1\BNA_F\Data\BF022615\
Data File : BF077460.D
Acq On : 26 Feb 2015 11:36
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 05:51:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 27 07:02:57 2015
Response via : Initial Calibration

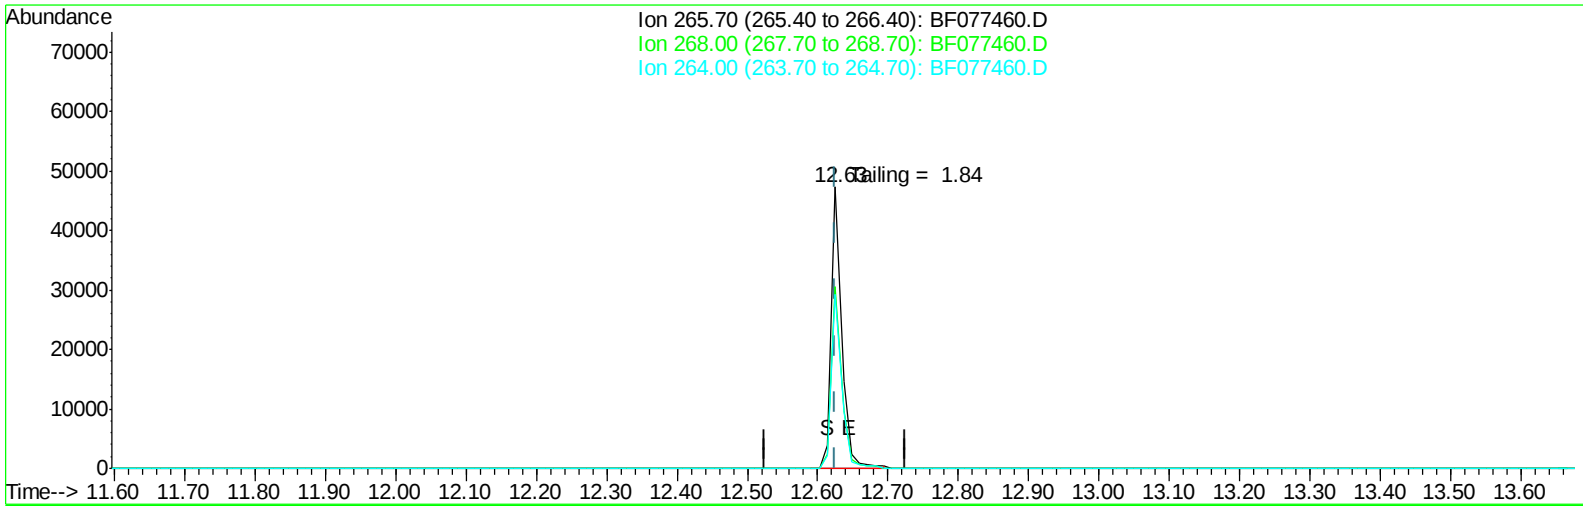

TIC: BF077460.D

(69) Pentachlorophenol (C)




12.629min (+0.004) 0.00ng

response 48112

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	64.40
264.00	63.40	61.92
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF022615\
Data File : BF077460.D
Acq On : 26 Feb 2015 11:36
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 05:51:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 27 07:02:57 2015
Response via : Initial Calibration

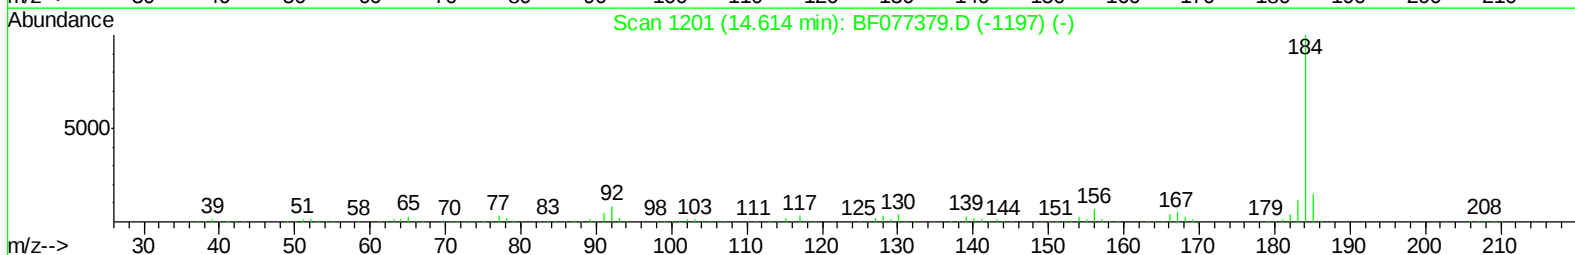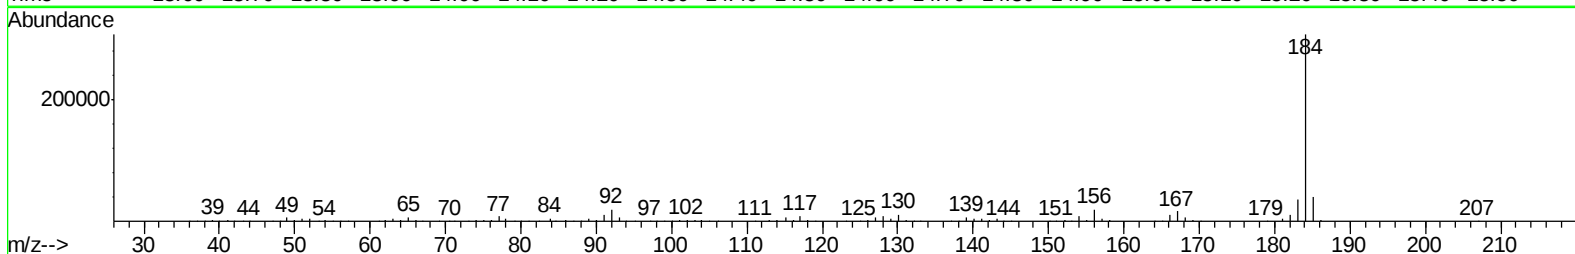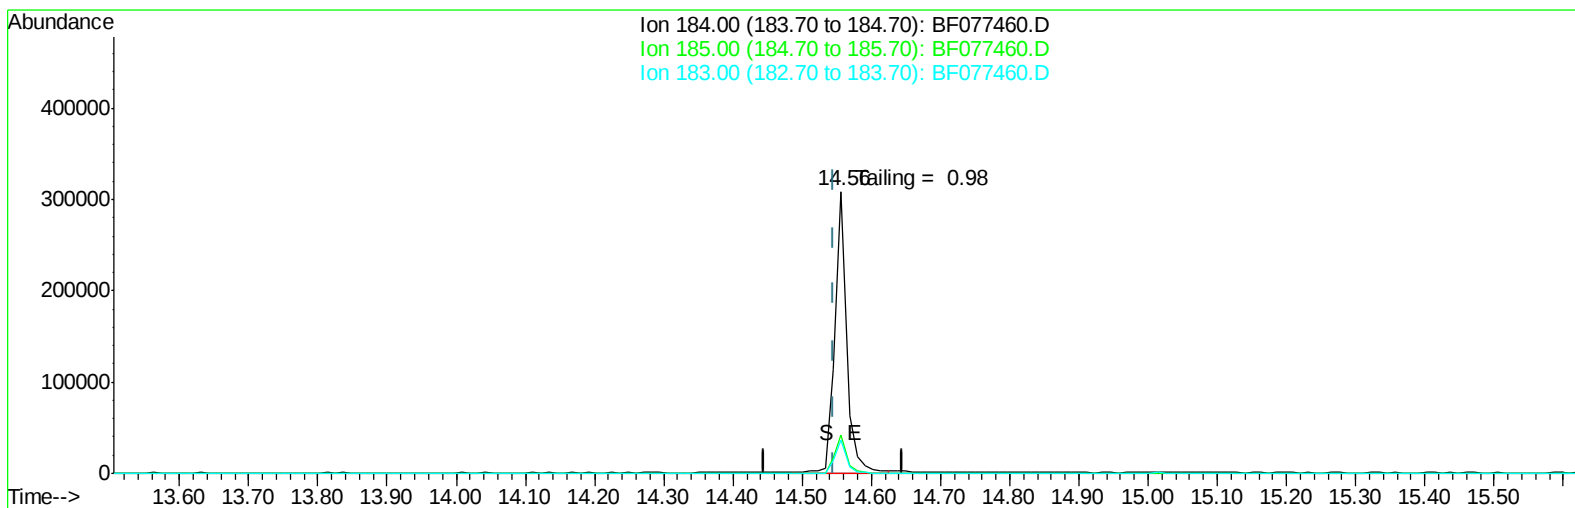

TIC: BF077460.D

(76) Benzidine

14.557min (+0.012) 43727.91ng

response 354571

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.45
183.00	11.60	11.65
0.00	0.00	0.00