

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022615\
 Data File : BF077494.D
 Acq On : 27 Feb 2015 6:54
 Operator : TP/IZ
 Sample : G1385-16
 Misc : S
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-16-D11

Quant Time: Feb 27 11:51:00 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 27 07:02:57 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.27	152	71140	20.00	ng	0.00
21) Naphthalene-d8	8.85	136	303265	20.00	ng	0.00
38) Acenaphthene-d10	11.02	164	167334	20.00	ng	0.00
63) Phenanthrene-d10	12.87	188	330503	20.00	ng	0.00
75) Chrysene-d12	16.17	240	362317	20.00	ng	0.02
86) Perylene-d12	17.95	264	366248	20.00	ng	0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	274213	64.35	ng	0.01
7) Phenol-d6	6.83	99	376314	68.68	ng	0.00
23) Nitrobenzene-d5	7.96	82	214736	44.03	ng	0.00
41) 2,4,6-Tribromophenol	12.00	330	101838	63.21	ng	0.00
44) 2-Fluorobiphenyl	10.19	172	518195	48.29	ng	0.00
78) Terphenyl-d14	14.86	244	654677	42.24	ng	0.00
Target Compounds						Qvalue
31) Naphthalene	8.87	128	50970	3.36	ng	97
37) 2-Methylnaphthalene	9.73	142	26119	2.43	ng	98
49) Dimethylphthalate	10.70	163	31666	2.69	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022615\
Data File : BF077494.D
Acq On : 27 Feb 2015 6:54
Operator : TP/IZ
Sample : G1385-16
Misc : S
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-16-D11

Quant Time: Feb 27 11:51:00 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 27 07:02:57 2015
Response via : Initial Calibration




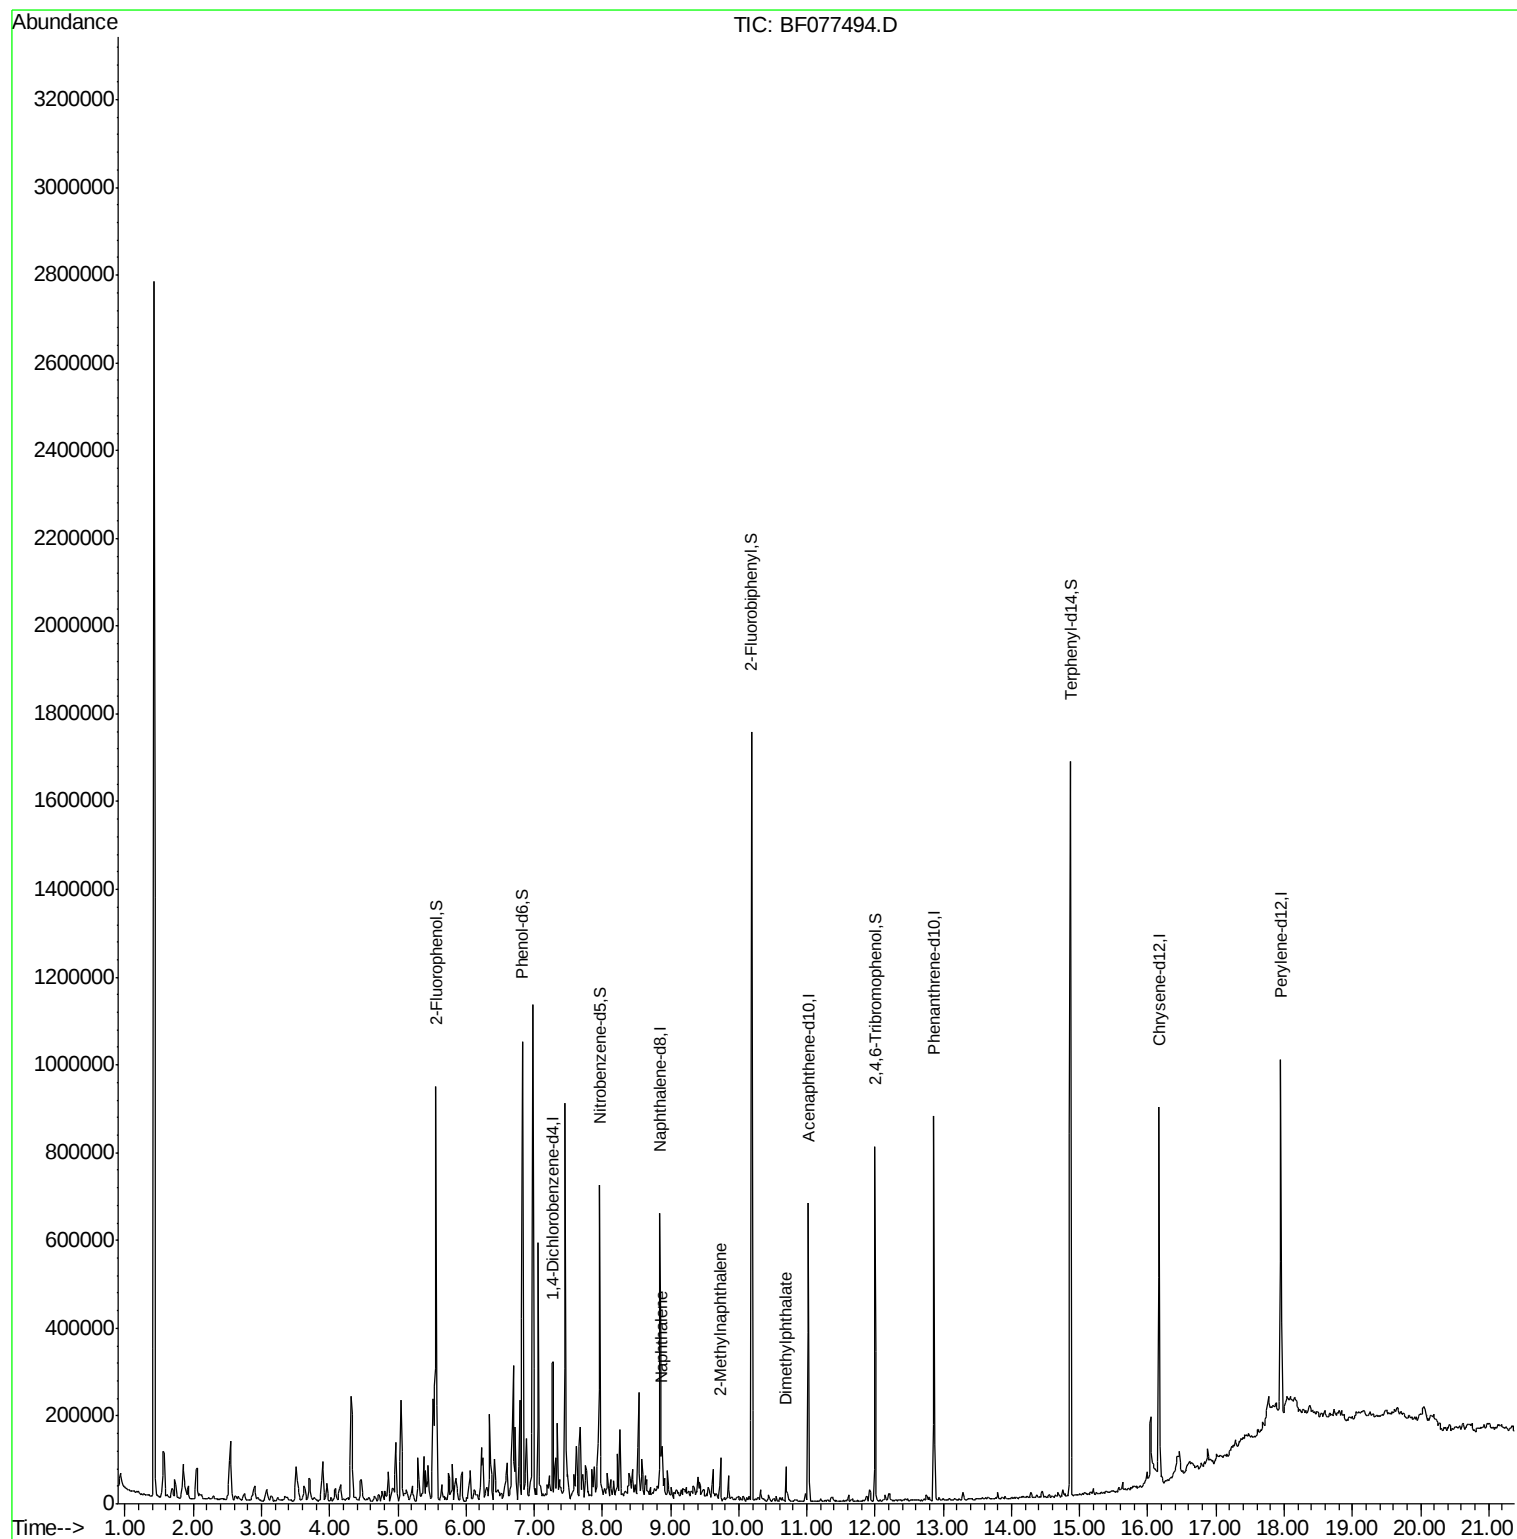


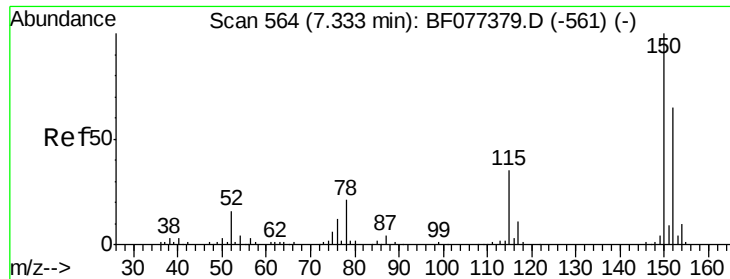

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.27 min Scan# 559
 Delta R.T. 0.01 min
 Lab File: BF077494.D
 Acq: 27 Feb 2015 6:54




Instrument :
 BNA_F
 ClientSampleId :
 B-16-D11

Tgt Ion:152 Resp: 71140
 Ion Ratio Lower Upper
 152 100
 150 149.6 124.0 186.0
 115 50.1 49.4 74.2

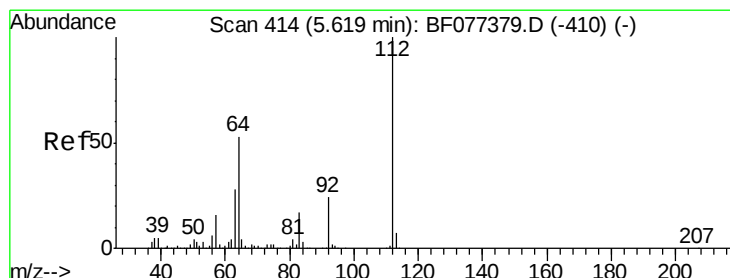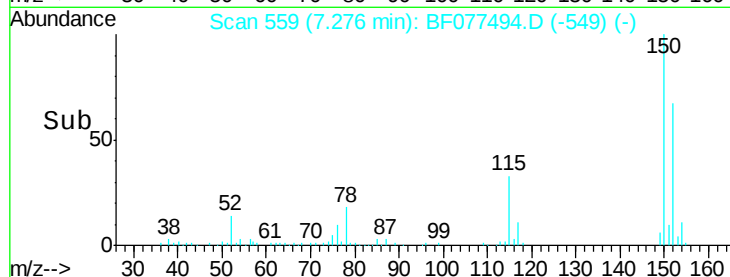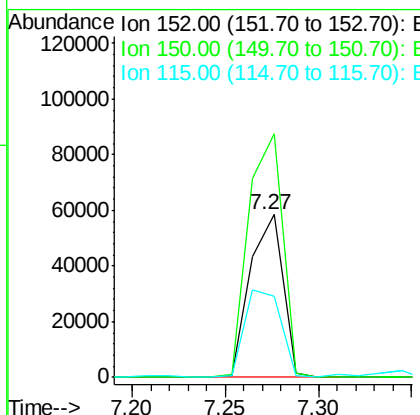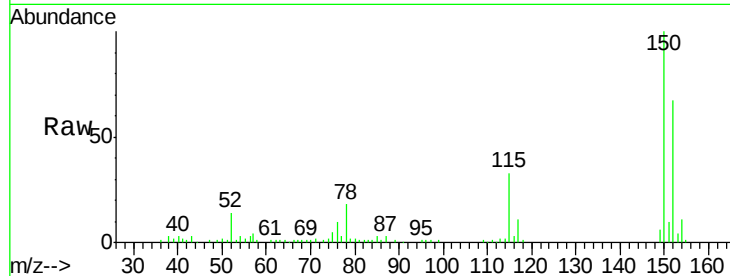

#5
 2-Fluorophenol
 Concen: 64.35 ng
 RT: 5.56 min Scan# 409
 Delta R.T. 0.01 min
 Lab File: BF077494.D
 Acq: 27 Feb 2015 6:54

Tgt Ion:112 Resp: 274213
 Ion Ratio Lower Upper
 112 100
 64 58.7 48.5 72.7
 63 30.5 25.0 37.4

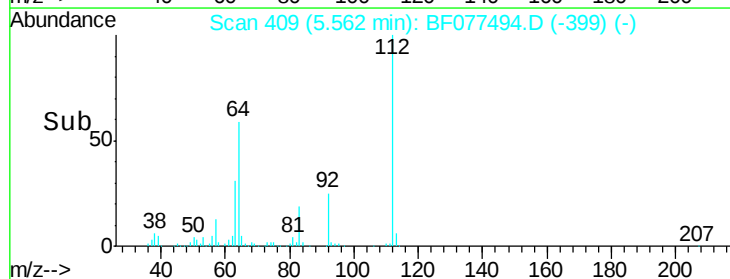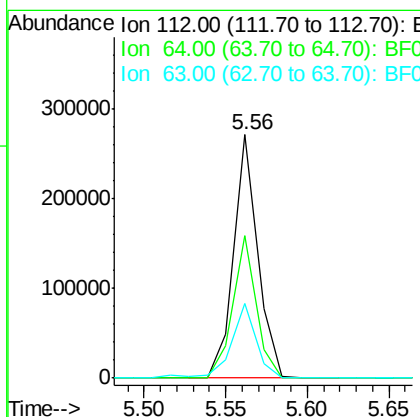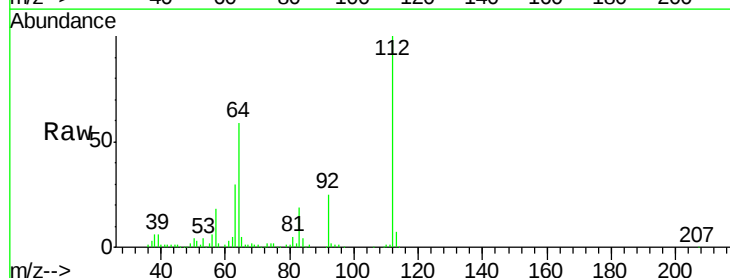



#7

Phenol-d6

Concen: 68.68 ng

RT: 6.83 min Scan# 520

Delta R.T. 0.01 min

Lab File: BF077494.D

Acq: 27 Feb 2015 6:54

Instrument :

BNA_F

ClientSampleId :

B-16-D11


Tgt Ion: 99 Resp: 376314

Ion Ratio Lower Upper

99 100

42 16.4 16.2 24.4




71 31.3 26.7 40.1



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

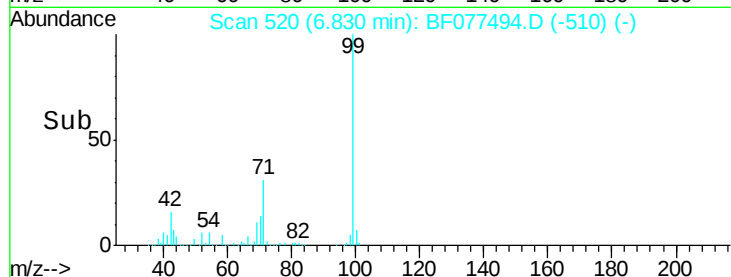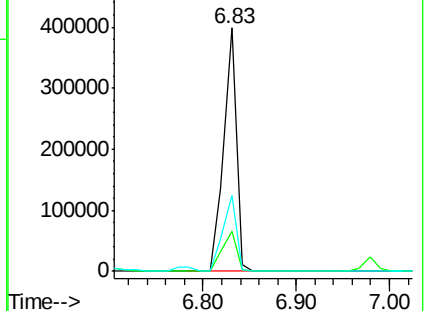

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.85 min Scan# 696

Delta R.T. 0.00 min

Lab File: BF077494.D

Acq: 27 Feb 2015 6:54

Tgt Ion: 136 Resp: 303265


Ion Ratio Lower Upper

136 100

137 11.0 8.6 13.0

54 8.4 6.2 9.4

68 6.4 5.0 7.6






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

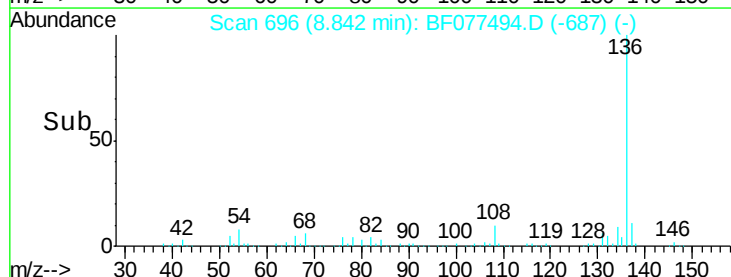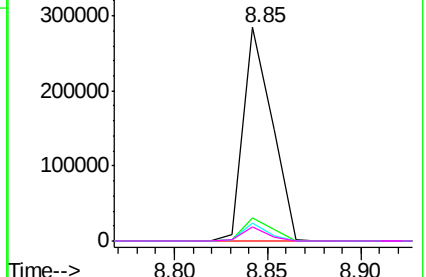


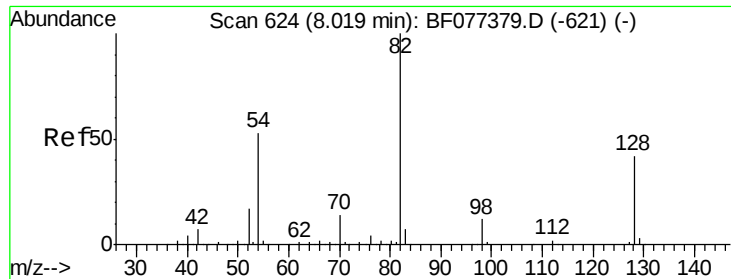




#23
 Nitrobenzene-d5
 Concen: 44.03 ng
 RT: 7.96 min Scan# 619
 Delta R.T. -0.00 min
 Lab File: BF077494.D
 Acq: 27 Feb 2015 6:54

Instrument :
 BNA_F
 ClientSampleId :
 B-16-D11

Tgt Ion	Ratio	Lower	Upper
82	100		
128	50.9	43.8	65.8
54	47.4	36.7	55.1

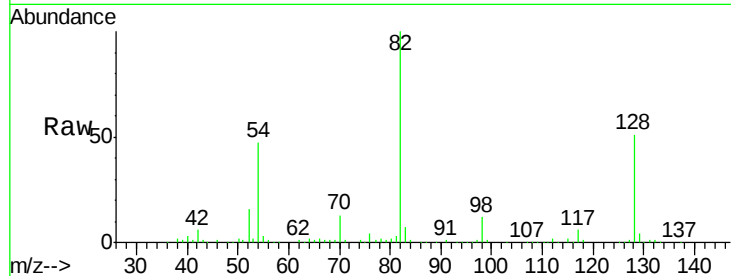


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

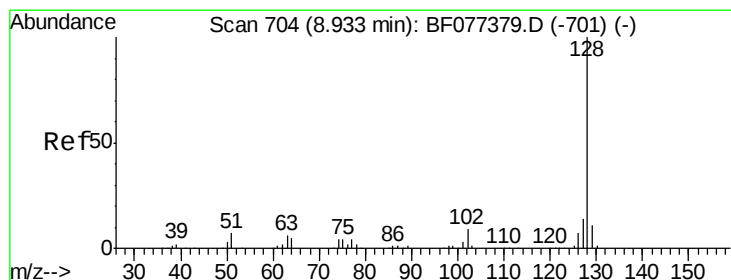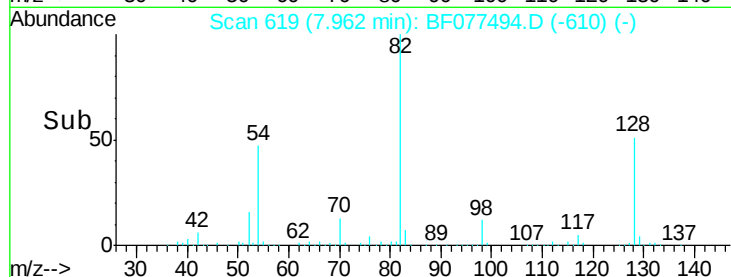
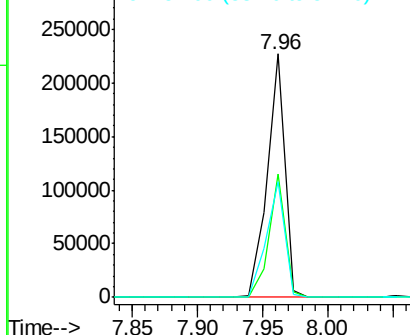



#31
 Naphthalene
 Concen: 3.36 ng
 RT: 8.87 min Scan# 698
 Delta R.T. 0.01 min
 Lab File: BF077494.D
 Acq: 27 Feb 2015 6:54

Tgt Ion	Ratio	Lower	Upper
128	100		
129	12.0	9.4	14.0
127	15.3	10.6	15.8



Abundance Ion 128.00 (127.70 to 128.70): E
 Ion 129.00 (128.70 to 129.70): E
 Ion 127.00 (126.70 to 127.70): E

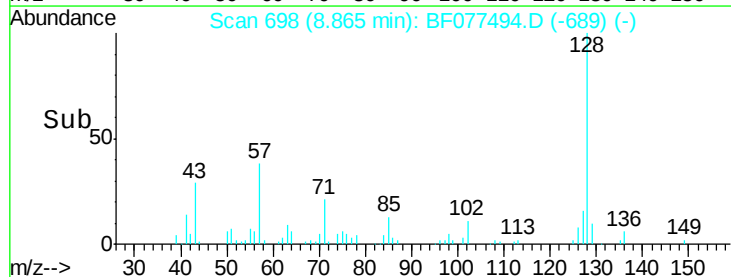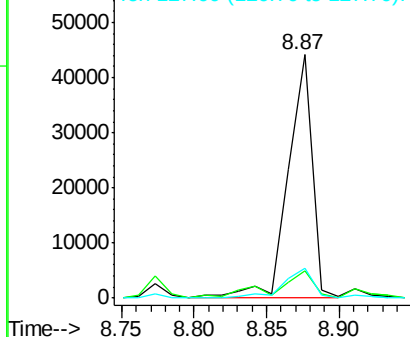


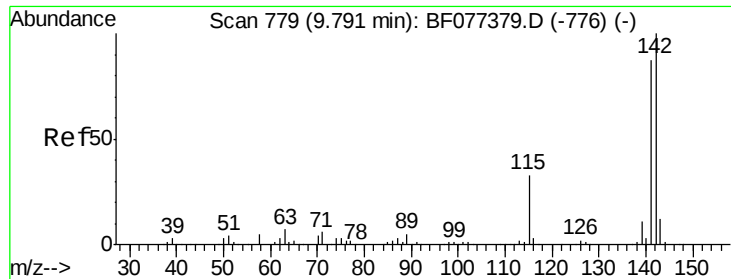




#37
 2-Methylnaphthalene
 Concen: 2.43 ng
 RT: 9.73 min Scan# 774
 Delta R.T. -0.00 min
 Lab File: BF077494.D
 Acq: 27 Feb 2015 6:54

Instrument :
 BNA_F
 ClientSampleId :
 B-16-D11

Tgt Ion:142 Resp: 26119
 Ion Ratio Lower Upper
 142 100
 141 90.1 70.7 106.1
 115 31.4 24.2 36.4

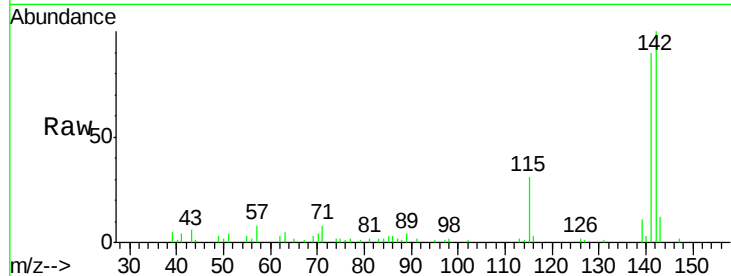


Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E
 Ion 115.00 (114.70 to 115.70): E

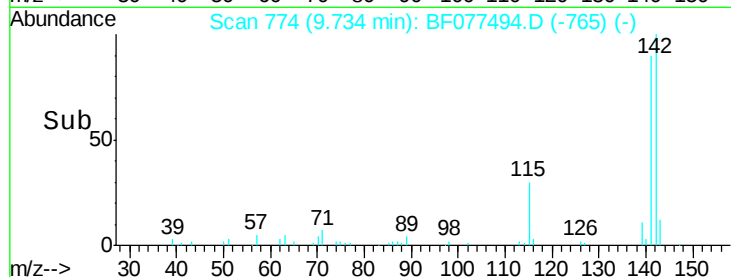
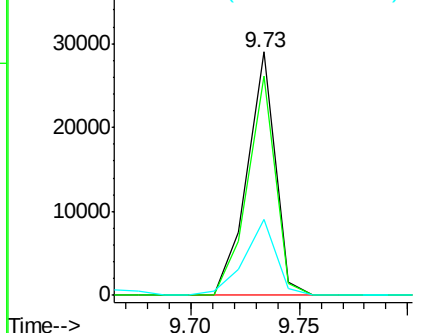


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 11.02 min Scan# 887
 Delta R.T. 0.01 min
 Lab File: BF077494.D
 Acq: 27 Feb 2015 6:54

Tgt Ion:164 Resp: 167334
 Ion Ratio Lower Upper
 164 100
 162 104.0 83.2 124.8
 160 45.7 34.6 52.0



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

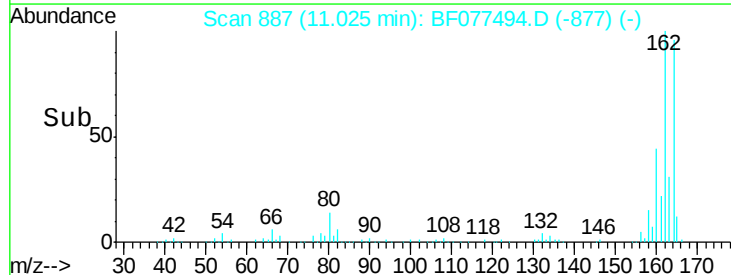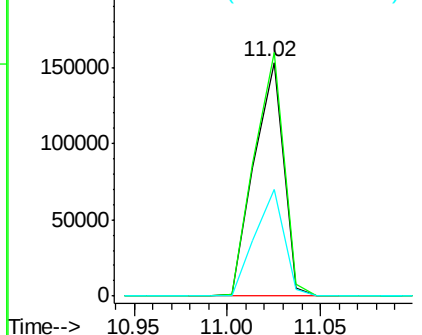







#41
 2,4,6-Tribromophenol
 Concen: 63.21 ng
 RT: 12.00 min Scan# 973
 Delta R.T. 0.01 min
 Lab File: BF077494.D
 Acq: 27 Feb 2015 6:54

Instrument :
 BNA_F
 ClientSampleId :
 B-16-D11

Tgt Ion:330 Resp: 101838
 Ion Ratio Lower Upper
 330 100
 332 97.1 77.4 116.2
 141 38.8 28.8 43.2

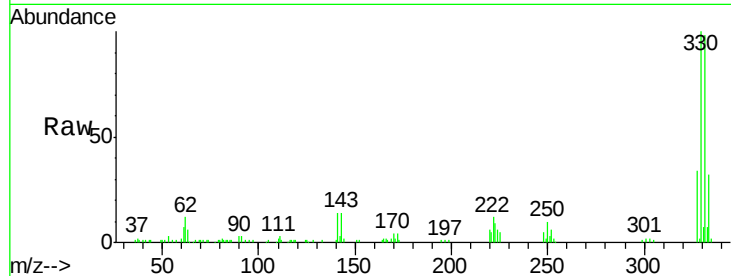


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

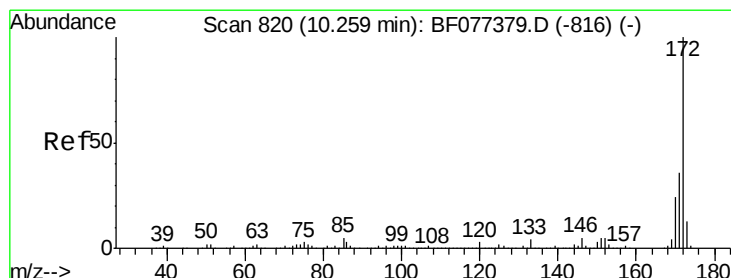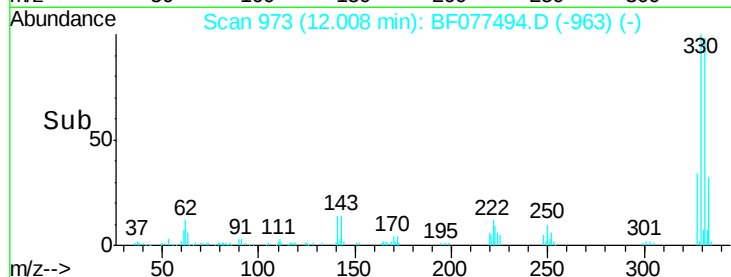
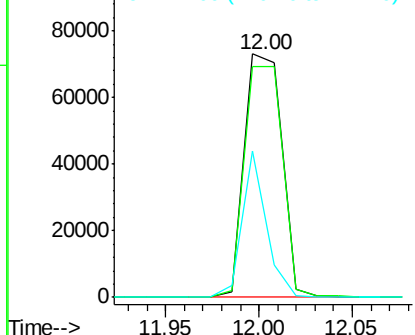



#44
 2-Fluorobiphenyl
 Concen: 48.29 ng
 RT: 10.19 min Scan# 814
 Delta R.T. 0.00 min
 Lab File: BF077494.D
 Acq: 27 Feb 2015 6:54

Tgt Ion:172 Resp: 518195
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.9 43.3
 170 23.9 19.4 29.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

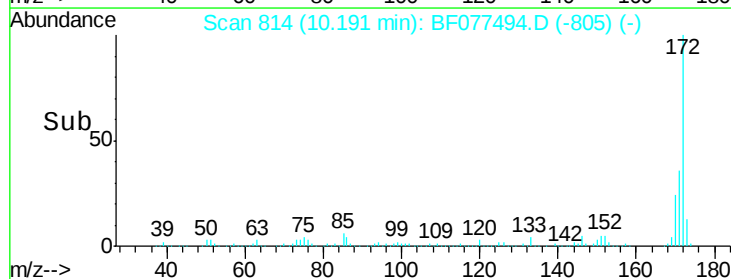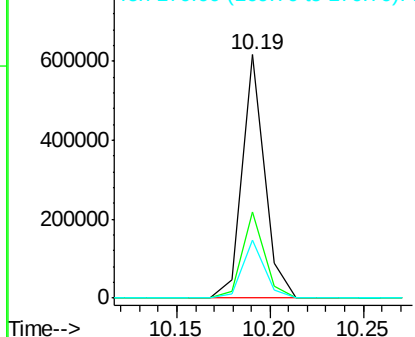

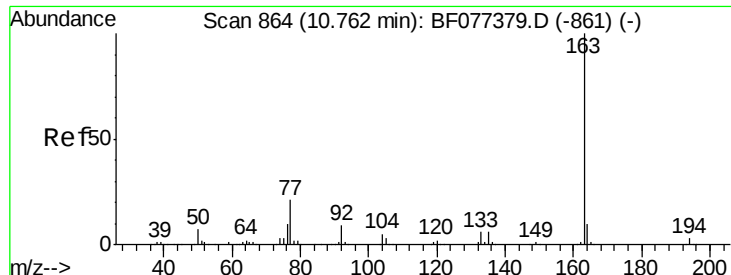

#49

Dimethylphthalate

Concen: 2.69 ng

RT: 10.70 min Scan# 858

Delta R.T. -0.01 min

Lab File: BF077494.D

Acq: 27 Feb 2015 6:54

Instrument :

BNA_F

ClientSampleId :

B-16-D11


Tgt Ion:163 Resp: 31666

Ion Ratio Lower Upper

163 100

194 4.1 2.6 4.0#




164 9.5 8.6 13.0



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

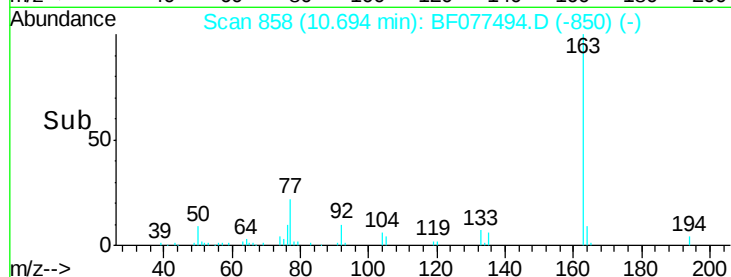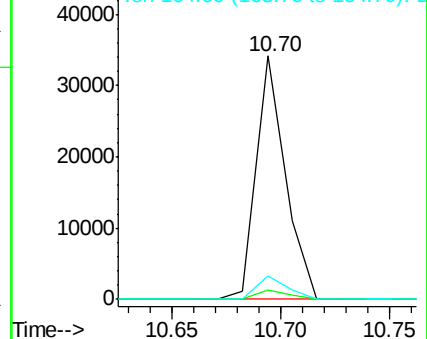

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.87 min Scan# 1048

Delta R.T. 0.00 min

Lab File: BF077494.D

Acq: 27 Feb 2015 6:54


Tgt Ion:188 Resp: 330503

Ion Ratio Lower Upper

188 100

94 8.6 7.4 11.2



80 9.7 8.0 12.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



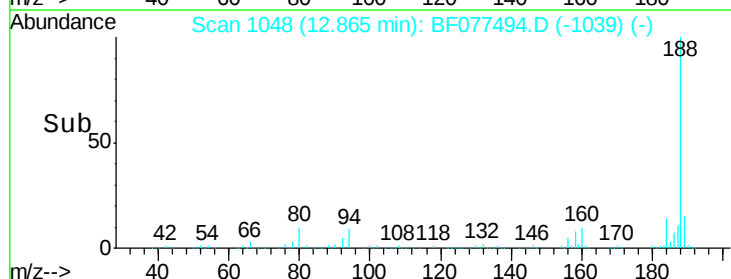
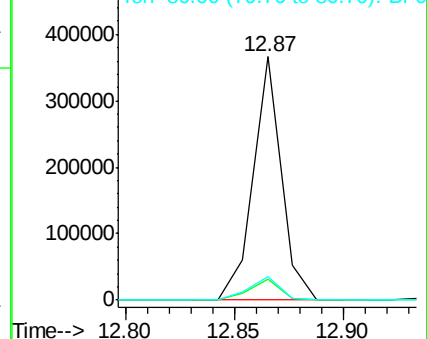


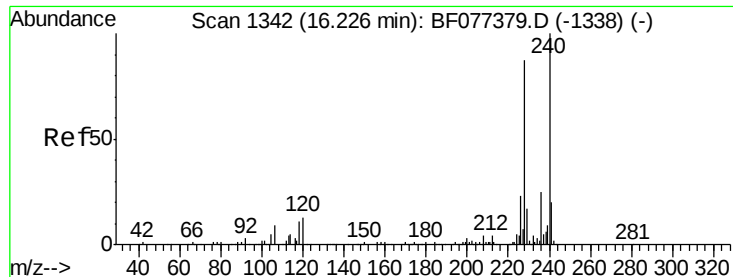

#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.17 min Scan# 1337
Delta R.T. 0.02 min
Lab File: BF077494.D
Acq: 27 Feb 2015 6:54




Instrument :
BNA_F
ClientSampleId :
B-16-D11




Tgt Ion:240 Resp: 362317
Ion Ratio Lower Upper
240 100
120 8.4 8.8 13.2#
236 25.7 20.7 31.1

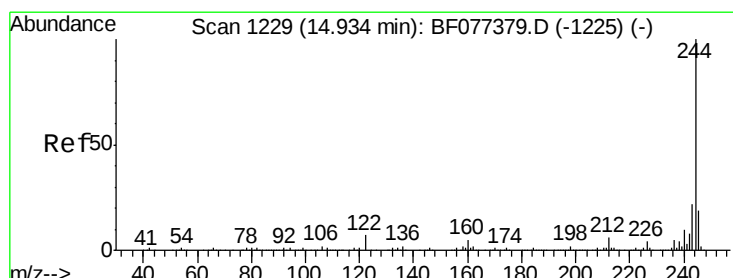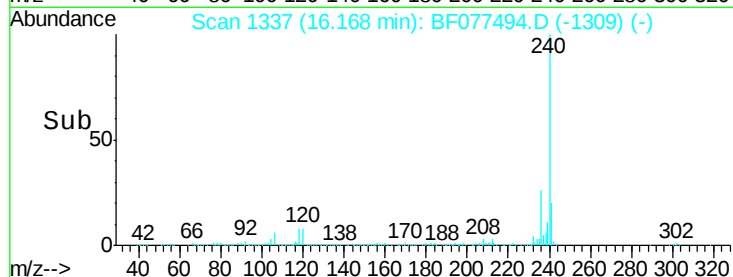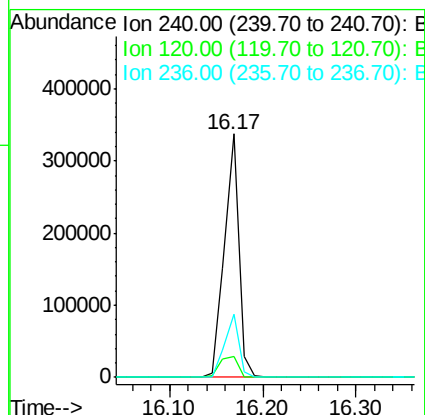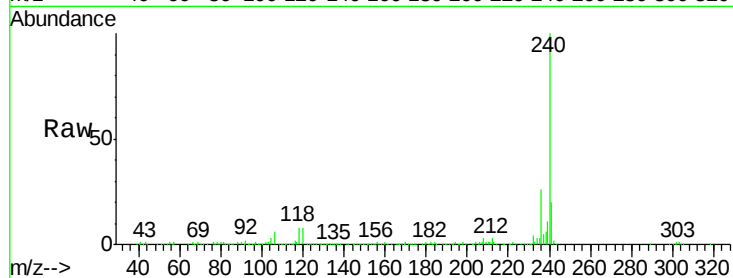

#78
Terphenyl-d14
Concen: 42.24 ng
RT: 14.86 min Scan# 1223
Delta R.T. 0.01 min
Lab File: BF077494.D
Acq: 27 Feb 2015 6:54

Tgt Ion:244 Resp: 654677
Ion Ratio Lower Upper
244 100
212 6.2 5.2 7.8
122 8.7 7.8 11.8

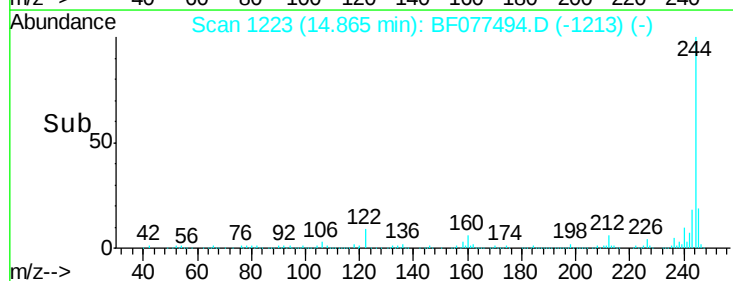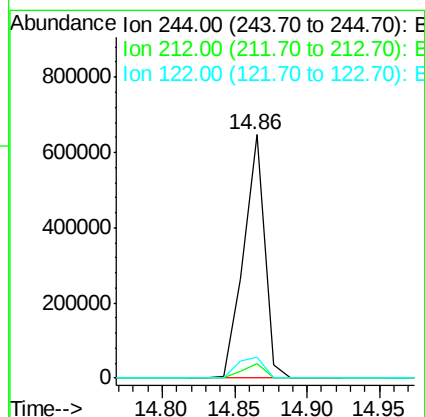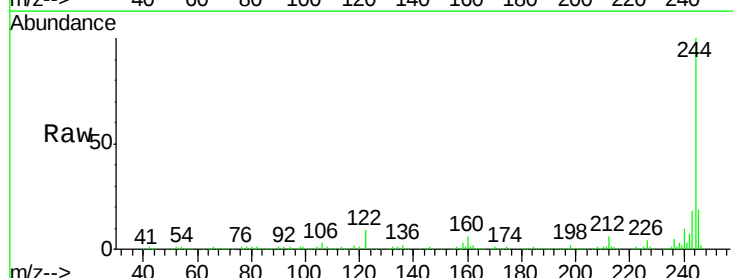

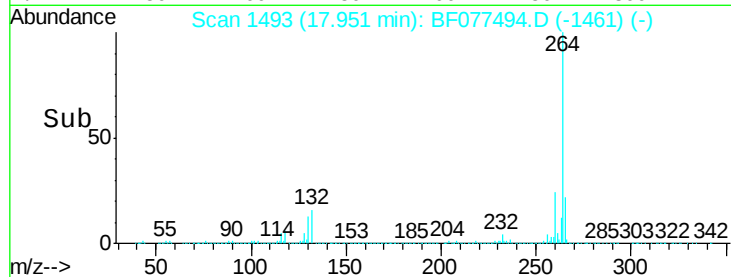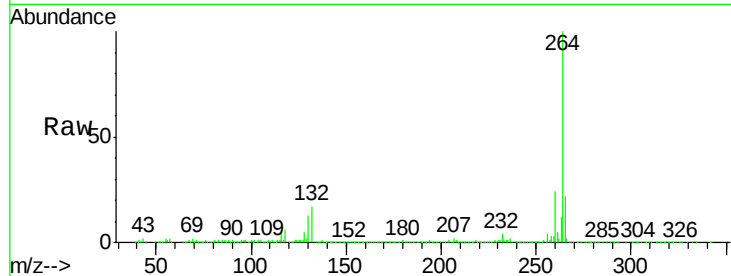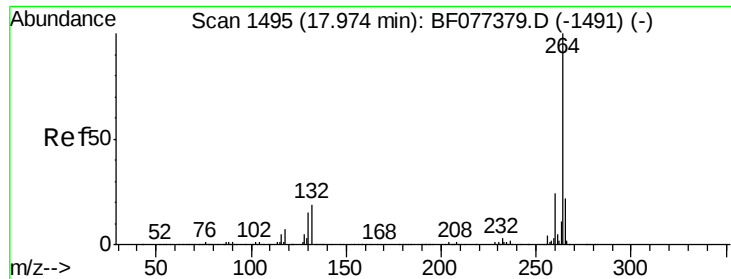

#86

Perylene-d12

Concen: 20.00 ng

RT: 17.95 min Scan# 1493

Delta R.T. 0.07 min

Lab File: BF077494.D

Acq: 27 Feb 2015 6:54

Instrument :

BNA_F

ClientSampleId :

B-16-D11

Tgt Ion: 264 Resp: 366248

Ion Ratio Lower Upper

264 100

260 23.9 19.3 28.9

265 21.7 16.8 25.2

