


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022615\
 Data File : BF077481.D
 Acq On : 26 Feb 2015 23:48
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 27 07:02:57 2015

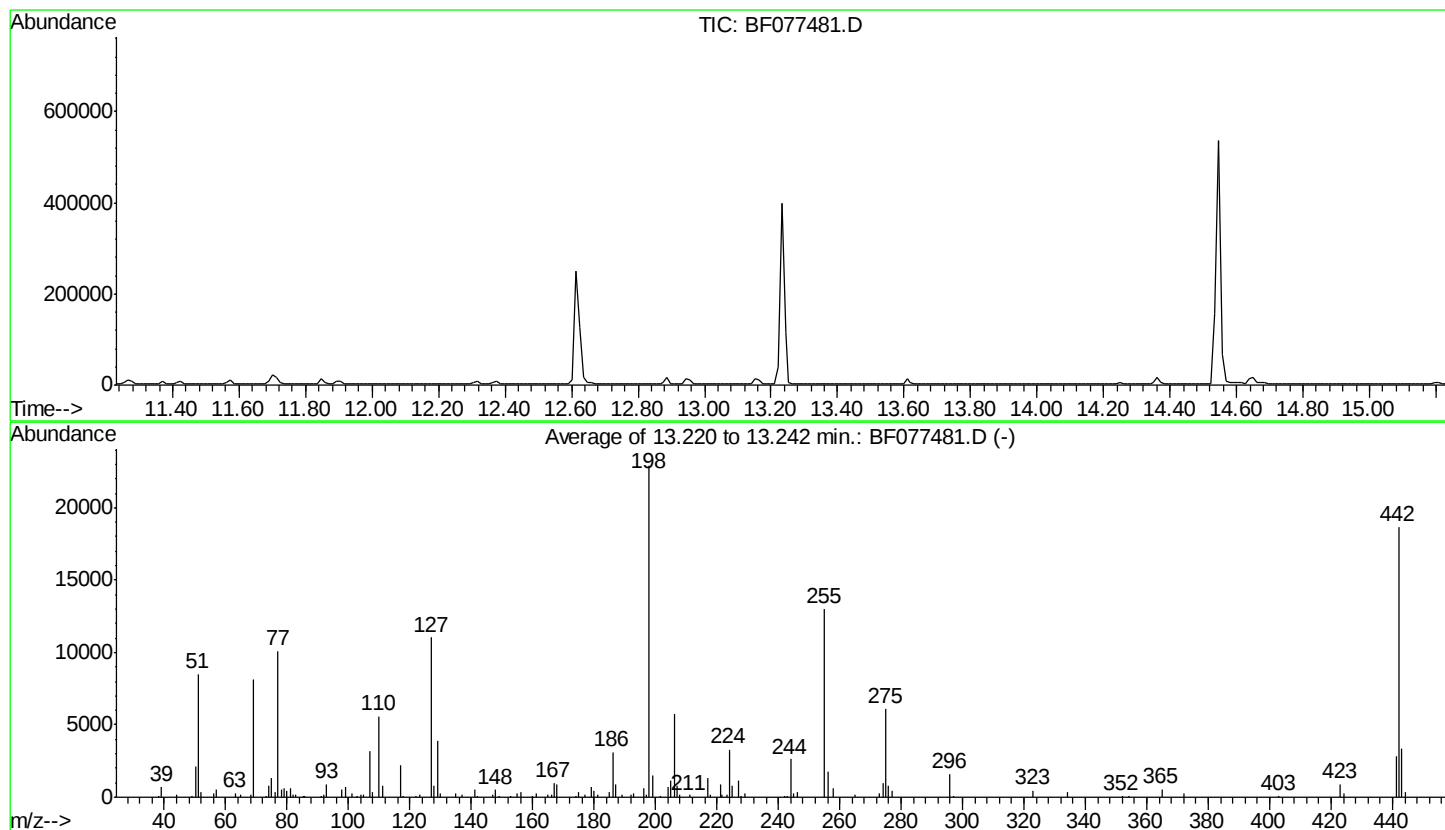

AutoFind: Scans 1079, 1080, 1081; Background Corrected with Scan 1076

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	8502	PASS
68	69	0.00	2	1.7	138	PASS
69	198	0.00	100	35.6	8150	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	11036	PASS
197	198	0.00	2	0.6	137	PASS
198	198	100	100	100.0	22907	PASS
199	198	5	9	6.8	1549	PASS
275	198	10	60	26.7	6123	PASS
365	198	1	100	2.5	563	PASS
441	442	0.01	24	15.3	2867	PASS
442	198	50	100	81.6	18702	PASS
443	442	15	24	18.0	3373	PASS