
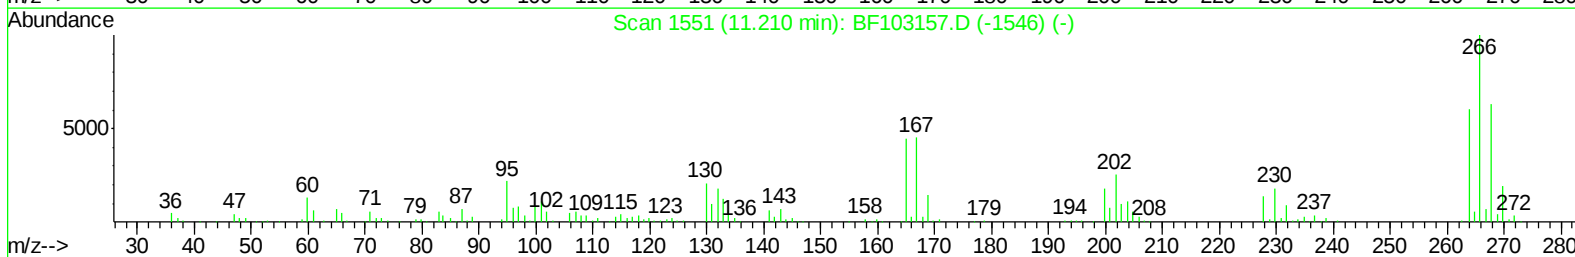
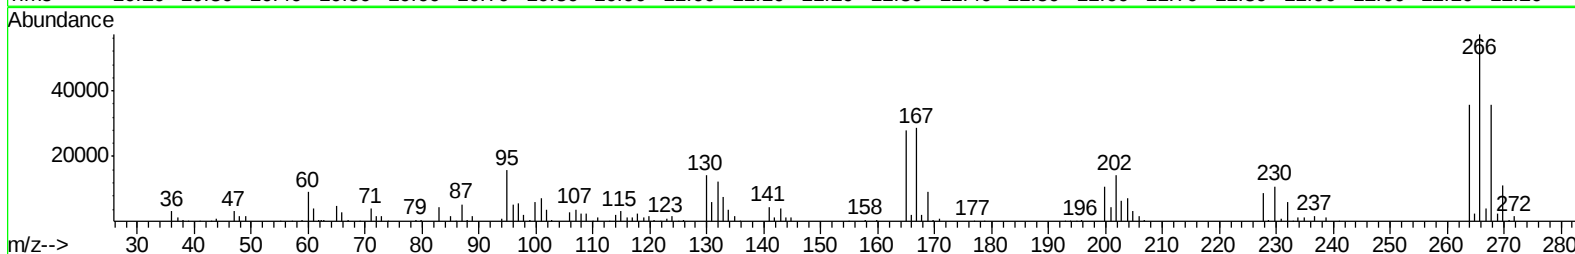


Data Path : Z:\HPCHEM1\BNA F\DATA\BF022618\
Data File : BF103204.D
Acq On : 26 Feb 2018 8:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 04:16:21 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 02:43:46 2018
Response via : Initial Calibration

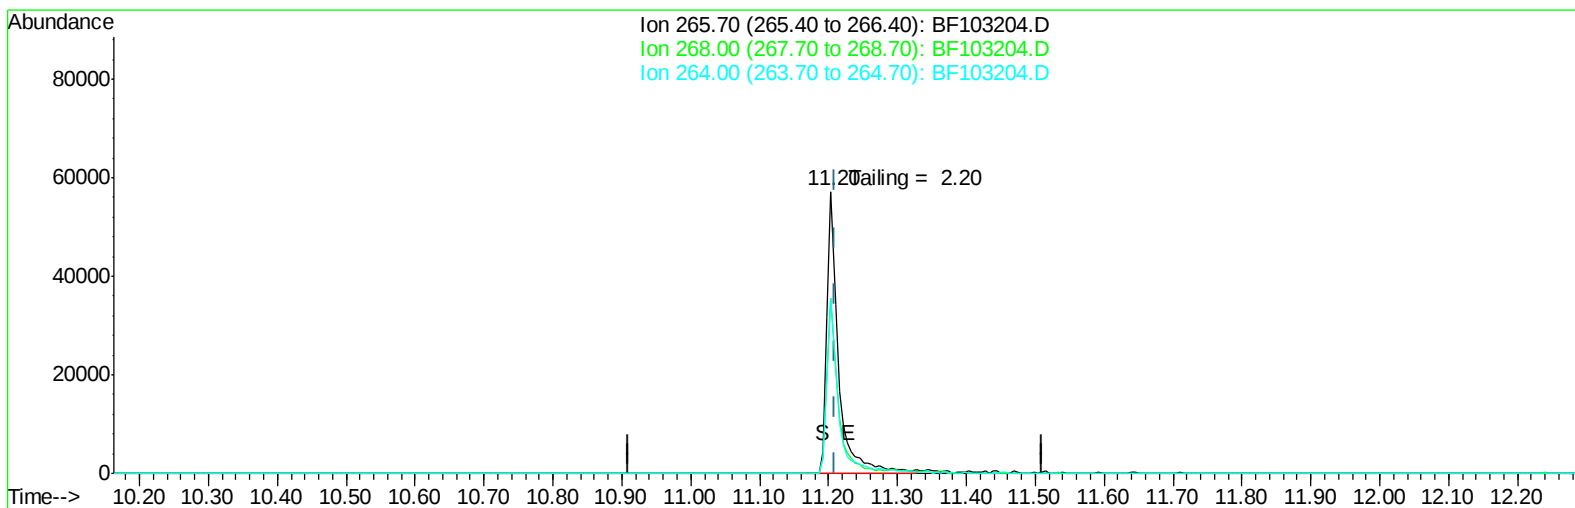

TIC: BF103204.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 109381.18ng

response 63984

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.23
264.00	61.90	62.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022618\
Data File : BF103204.D
Acq On : 26 Feb 2018 8:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 04:16:21 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 02:43:46 2018
Response via : Initial Calibration

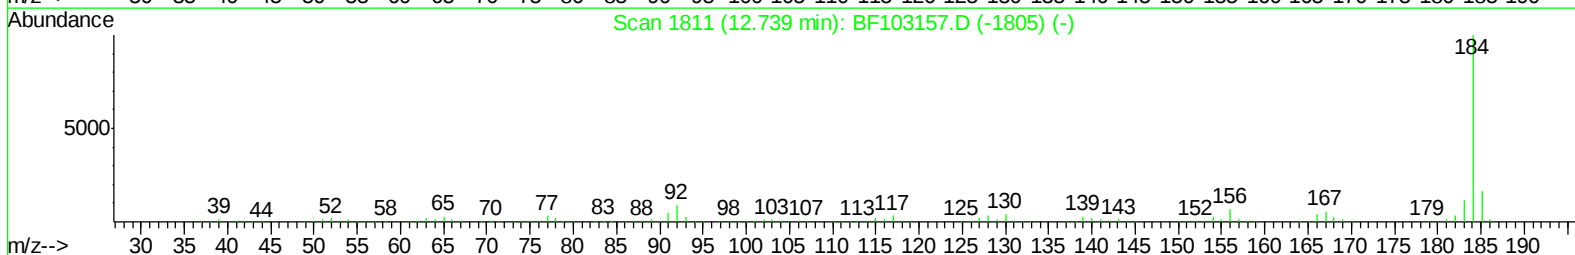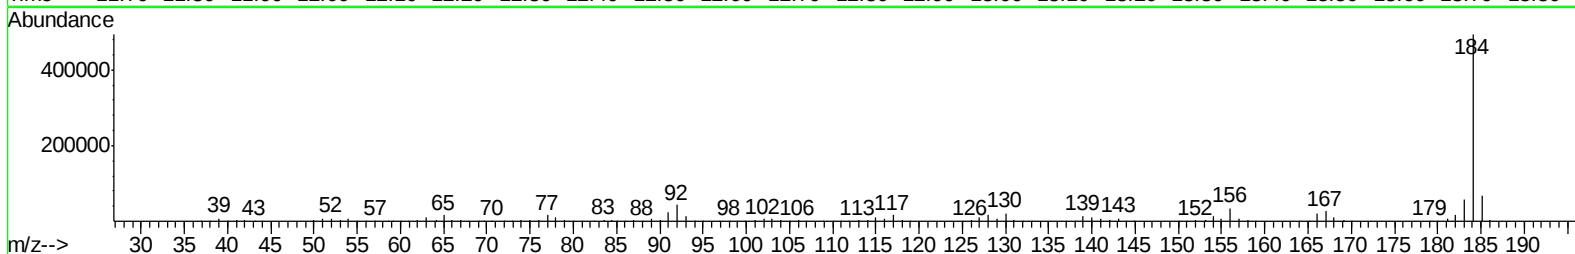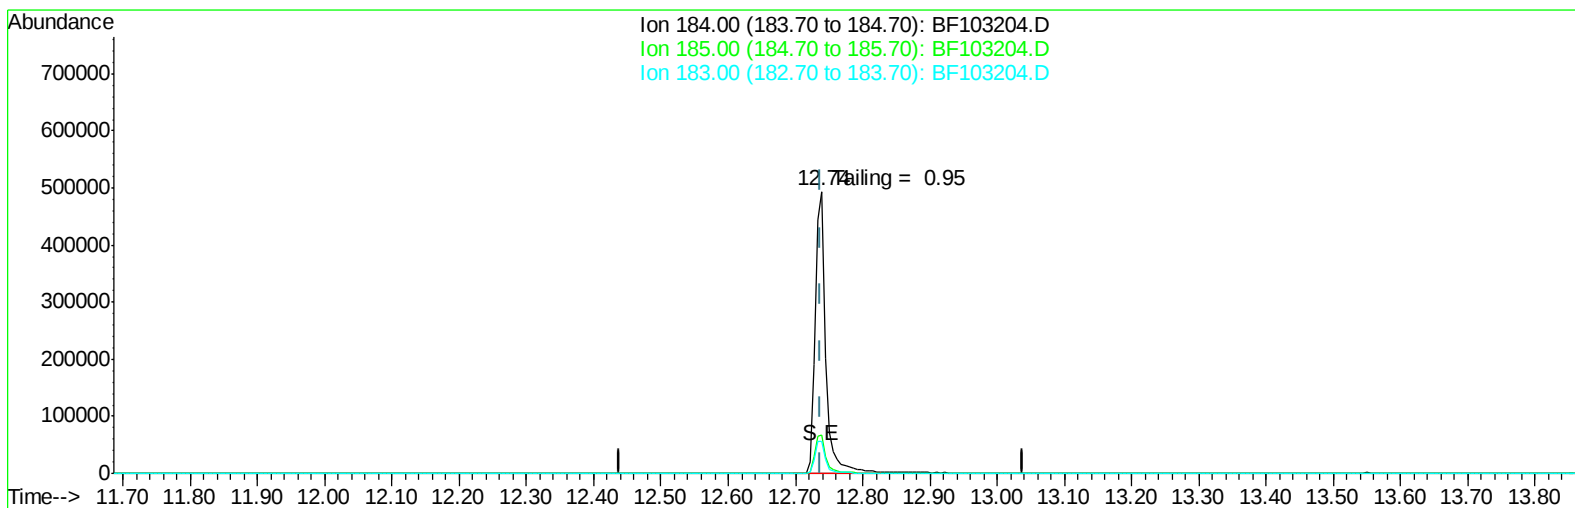

TIC: BF103204.D

(76) Benzidine

12.739min (-0.000) 23382.76ng

response 559469

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.85
183.00	11.60	11.46
0.00	0.00	0.00