


Data Path : Z:\HPCHEM1\BNA F\Data\BF022618\
 Data File : BF103204.D
 Acq On : 26 Feb 2018 8:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 23 02:43:46 2018

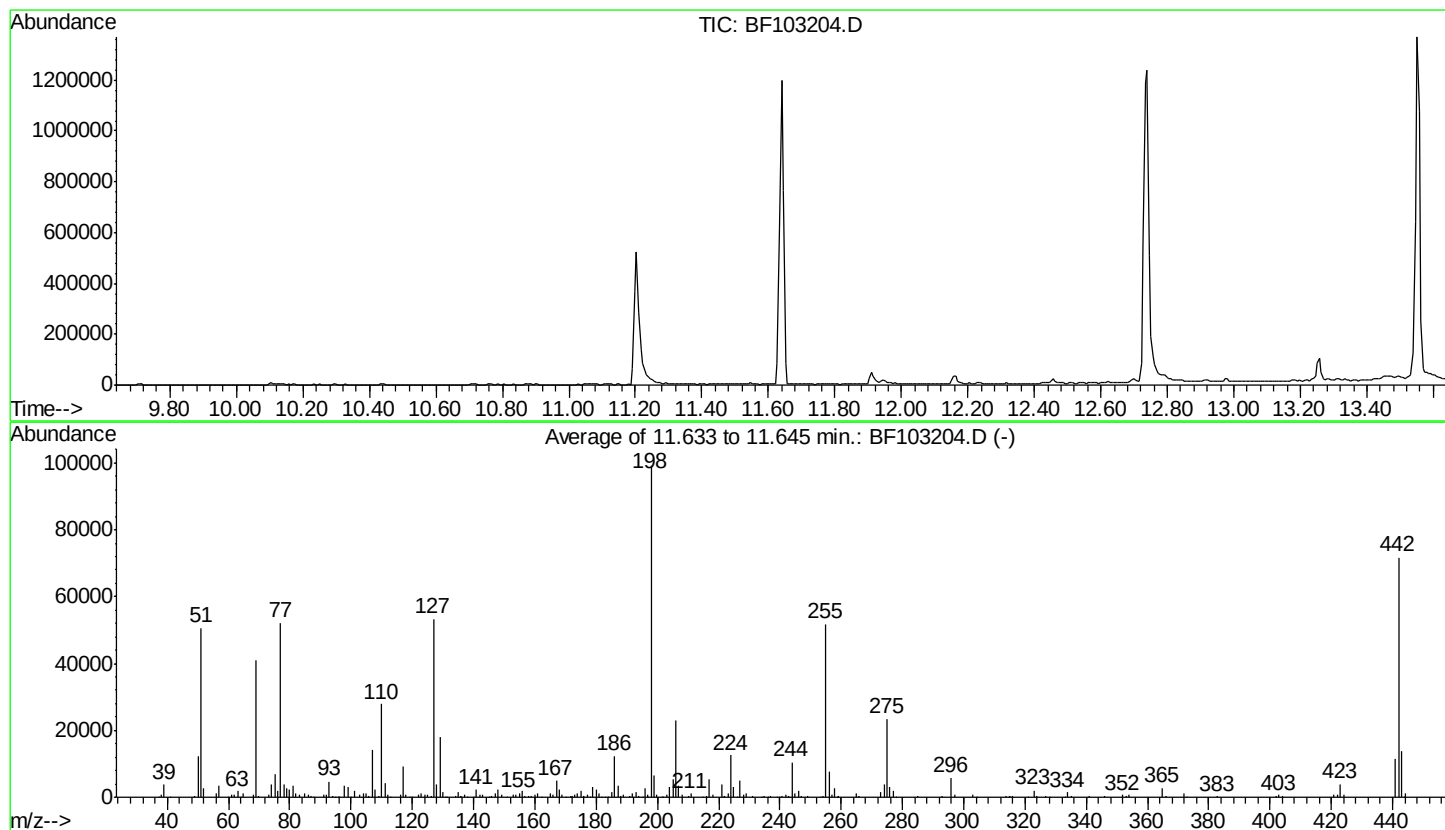

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.2	50744	PASS
68	69	0.00	2	1.8	732	PASS
69	198	0.00	100	41.3	40936	PASS
70	69	0.00	2	0.9	366	PASS
127	198	10	80	53.8	53328	PASS
197	198	0.00	2	0.9	939	PASS
198	198	100	100	100.0	99202	PASS
199	198	5	9	6.7	6607	PASS
275	198	10	60	23.6	23448	PASS
365	198	1	100	2.8	2794	PASS
441	443	0.01	100	84.3	11496	PASS
442	198	50	100	72.4	71781	PASS
443	442	15	24	19.0	13642	PASS