


Data Path : Z:\HPCHEM1\BNA_F\Data\BF022618\
 Data File : BF103220.D
 Acq On : 26 Feb 2018 16:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 23 02:43:46 2018

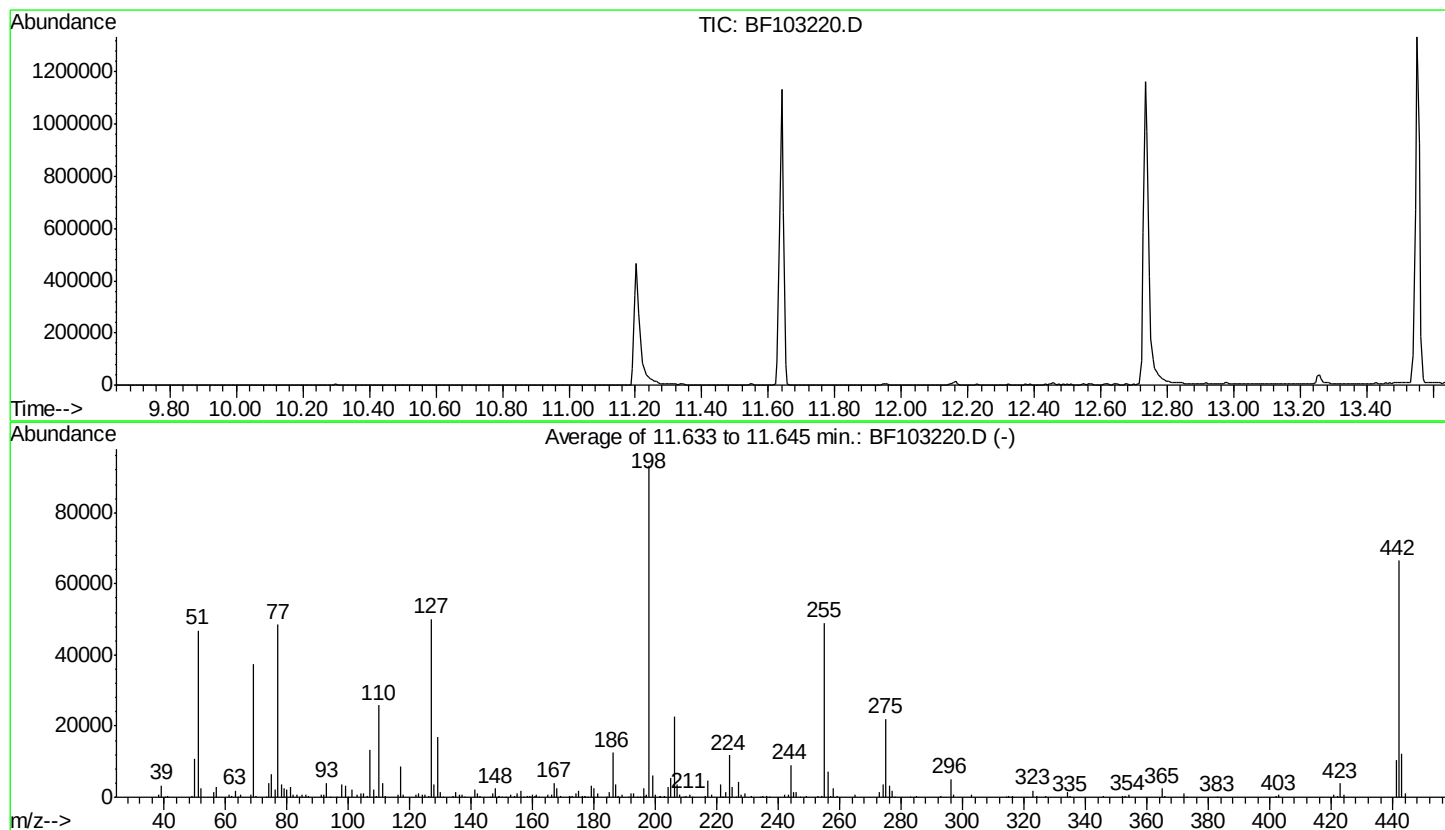

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	46837	PASS
68	69	0.00	2	1.7	645	PASS
69	198	0.00	100	40.2	37525	PASS
70	69	0.00	2	0.6	242	PASS
127	198	10	80	53.7	50048	PASS
197	198	0.00	2	0.8	753	PASS
198	198	100	100	100.0	93248	PASS
199	198	5	9	6.6	6195	PASS
275	198	10	60	23.6	22011	PASS
365	198	1	100	2.7	2480	PASS
441	443	0.01	100	85.6	10335	PASS
442	198	50	100	71.3	66450	PASS
443	442	15	24	18.2	12077	PASS