


Data Path : Z:\HPCHEM1\BNA F\Data\BF022618\
Data File : BF103247.D
Acq On : 27 Feb 2018 5:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 23 02:43:46 2018

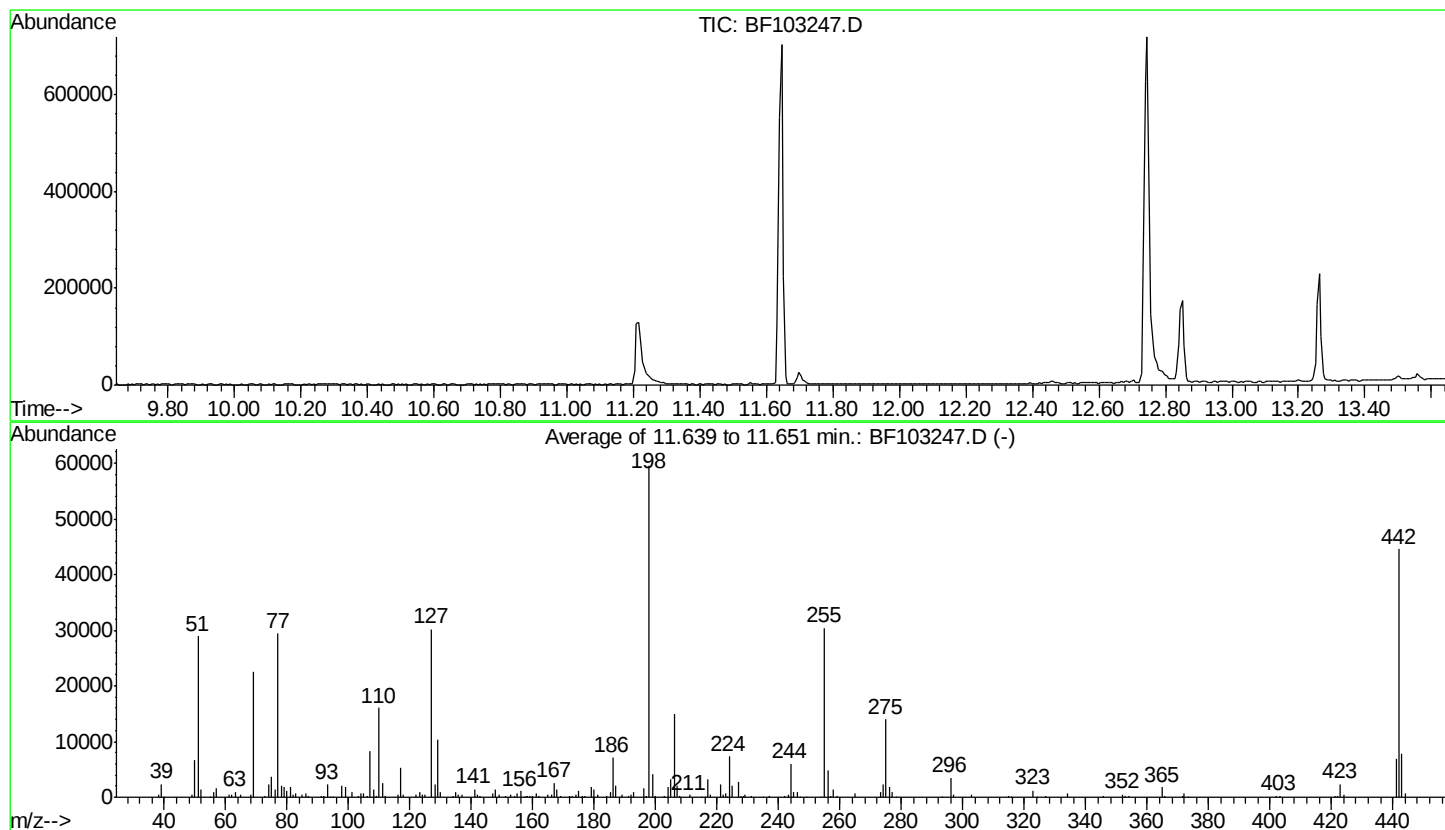

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.5	28909	PASS
68	69	0.00	2	1.8	414	PASS
69	198	0.00	100	37.7	22469	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	30211	PASS
197	198	0.00	2	0.4	231	PASS
198	198	100	100	100.0	59560	PASS
199	198	5	9	6.8	4067	PASS
275	198	10	60	23.5	13999	PASS
365	198	1	100	3.0	1788	PASS
441	443	0.01	100	86.5	6862	PASS
442	198	50	100	74.8	44552	PASS
443	442	15	24	17.8	7931	PASS