
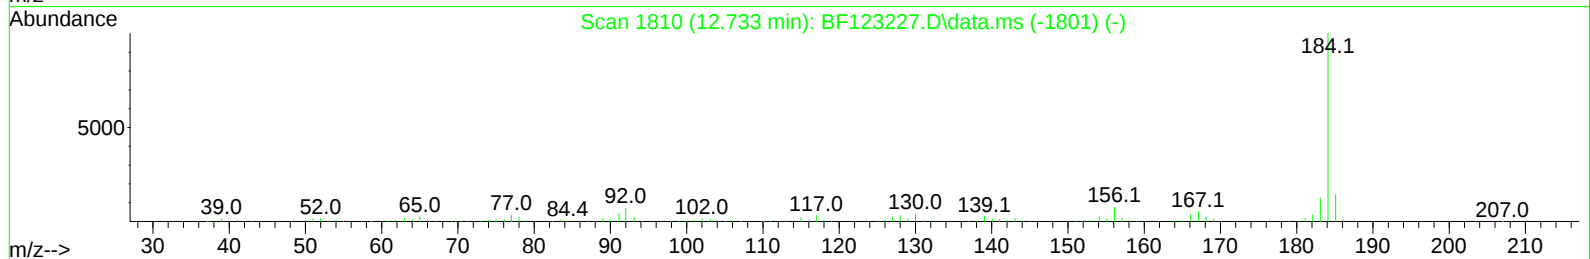
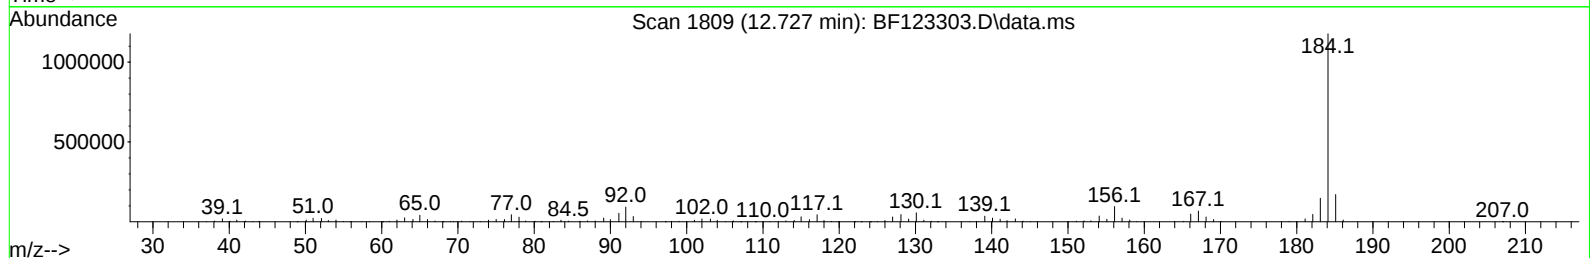


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022621\
Data File : BF123303.D
Acq On : 26 Feb 2021 14:28
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 15:25:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

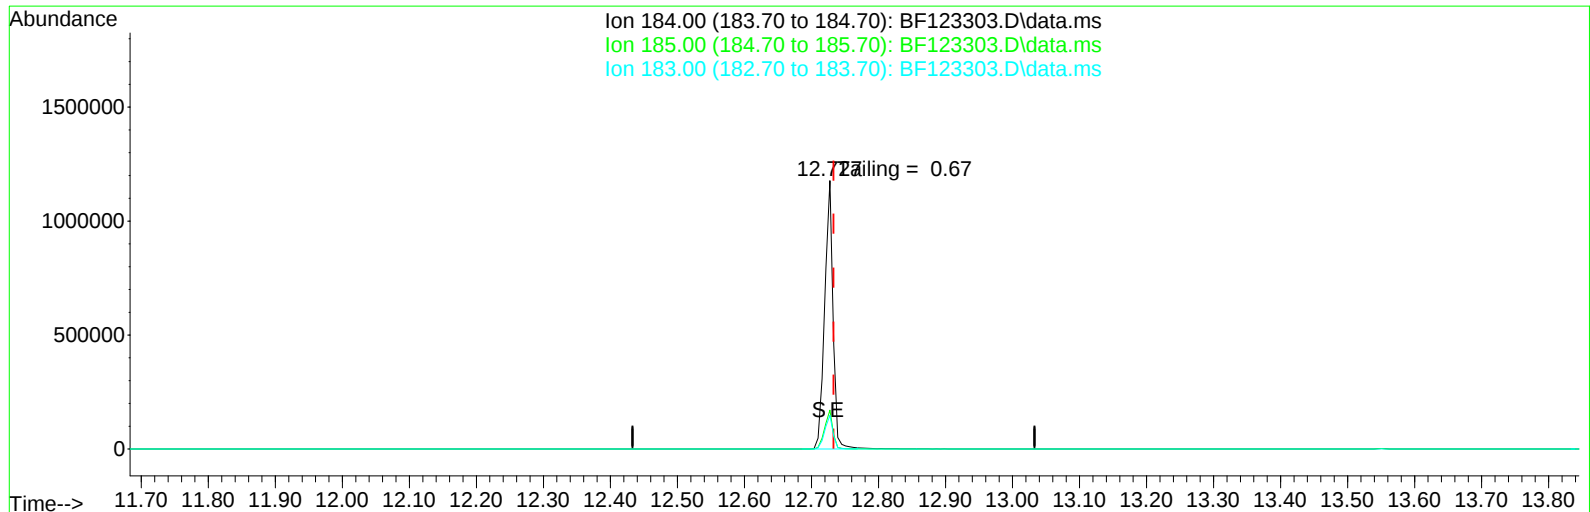

TIC: BF123303.D\data.ms

(77) Benzidine




12.727min (-0.006) 0.00 ng

response 1030495

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.50
183.00	12.10	12.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022621\
Data File : BF123303.D
Acq On : 26 Feb 2021 14:28
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 15:25:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

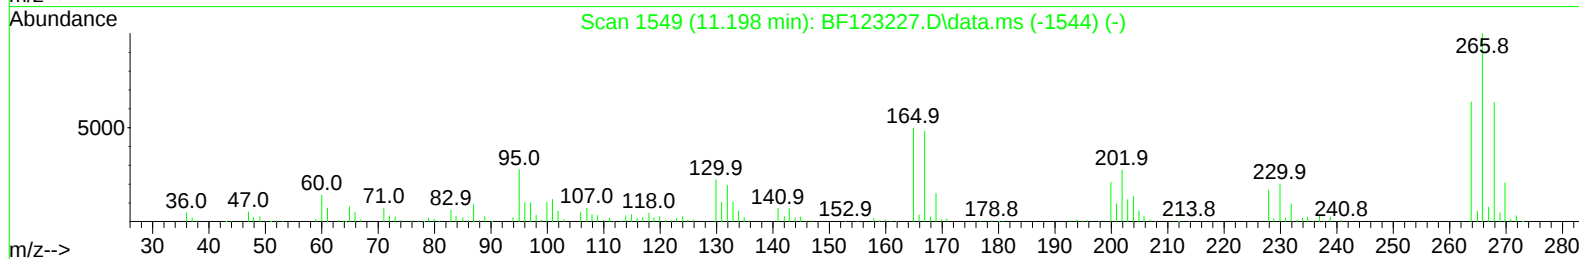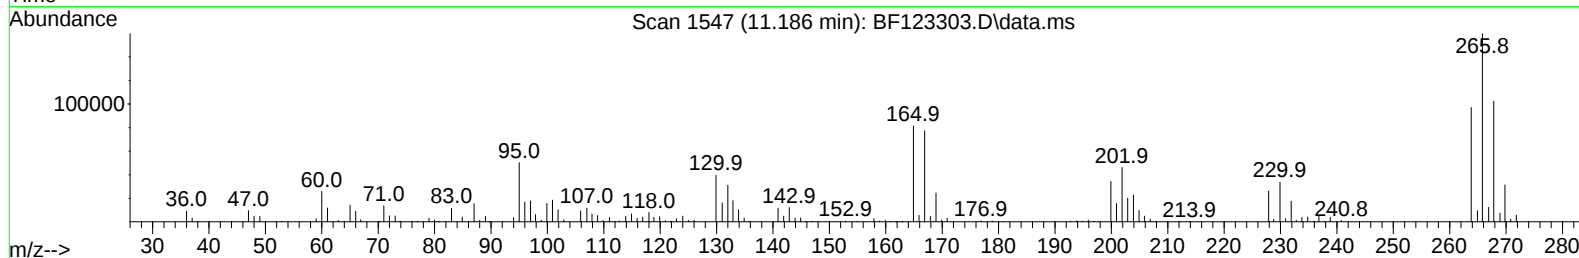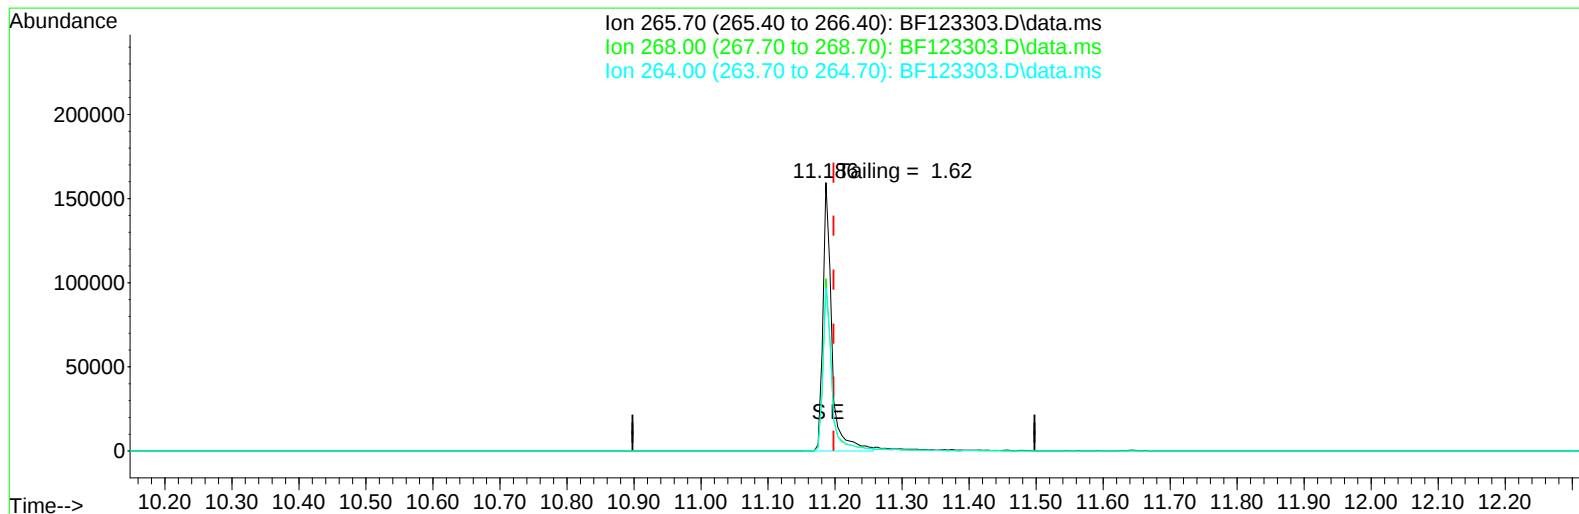

TIC: BF123303.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.012) 22908.21 ng

response 151167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.20
264.00	62.30	60.84
0.00	0.00	0.00