

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022621\
 Data File : BF123317.D
 Acq On : 26 Feb 2021 23:01
 Operator : JU/CG
 Sample : M1491-01 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SA-01-022521

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	570	573	588	rBV	524903	517870	41.52%	5.252%
2	6.475	743	746	757	rBV	581794	559204	44.83%	5.671%
3	6.845	806	809	813	rBV	946893	789523	63.29%	8.007%
4	7.404	901	904	916	rVB	389819	356981	28.62%	3.620%
5	8.134	1024	1028	1031	rBV	1310909	1047923	84.01%	10.628%
6	8.192	1035	1038	1041	rVB2	15023	17880	1.43%	0.181%
7	8.340	1059	1063	1065	rBV	25174	19731	1.58%	0.200%
8	8.557	1097	1100	1102	rBV	22080	17899	1.43%	0.182%
9	8.675	1116	1120	1124	rBV4	19123	20993	1.68%	0.213%
10	8.822	1142	1145	1148	rVB	13116	16419	1.32%	0.167%
11	9.157	1199	1202	1207	rBV3	28398	27231	2.18%	0.276%
12	9.210	1207	1211	1217	rBV	721236	655041	52.51%	6.643%
13	9.292	1221	1225	1228	rBV4	24550	32424	2.60%	0.329%
14	9.604	1275	1278	1282	rBV3	44843	61824	4.96%	0.627%
15	9.763	1301	1305	1307	rBV3	14896	18223	1.46%	0.185%
16	9.892	1323	1327	1330	rBV	1418674	1204547	96.57%	12.216%
17	10.545	1432	1438	1443	rVB2	16250	22134	1.77%	0.224%
18	10.681	1457	1461	1467	rBV	416779	394374	31.62%	4.000%
19	10.810	1478	1483	1486	rBV	23223	25563	2.05%	0.259%
20	11.245	1550	1557	1560	rBV6	7911	17442	1.40%	0.177%
21	11.380	1576	1580	1583	rBV	1575350	1247384	100.00%	12.651%
22	11.775	1643	1647	1649	rVB	27537	21820	1.75%	0.221%
23	11.910	1667	1670	1674	rBV	69480	74970	6.01%	0.760%
24	12.363	1744	1747	1750	rBV	42502	39013	3.13%	0.396%
25	12.463	1761	1764	1765	rBV2	39803	33738	2.70%	0.342%
26	12.480	1765	1767	1772	rVB	107500	96603	7.74%	0.980%
27	12.598	1784	1787	1790	rBV	50035	48214	3.87%	0.489%
28	12.698	1801	1804	1808	rBV5	20505	30100	2.41%	0.305%
29	12.827	1823	1826	1831	rVB	47686	57444	4.61%	0.583%
30	12.969	1846	1850	1853	rBV	825250	667001	53.47%	6.765%
31	14.027	2026	2030	2034	rBV	1005109	902769	72.37%	9.156%
32	15.504	2276	2281	2288	rVB	615729	817763	65.56%	8.294%


Sum of corrected areas: 9860045

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022621\
Data File : BF123317.D
Acq On : 26 Feb 2021 23:01
Operator : JU/CG
Sample : M1491-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SA-01-022521

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

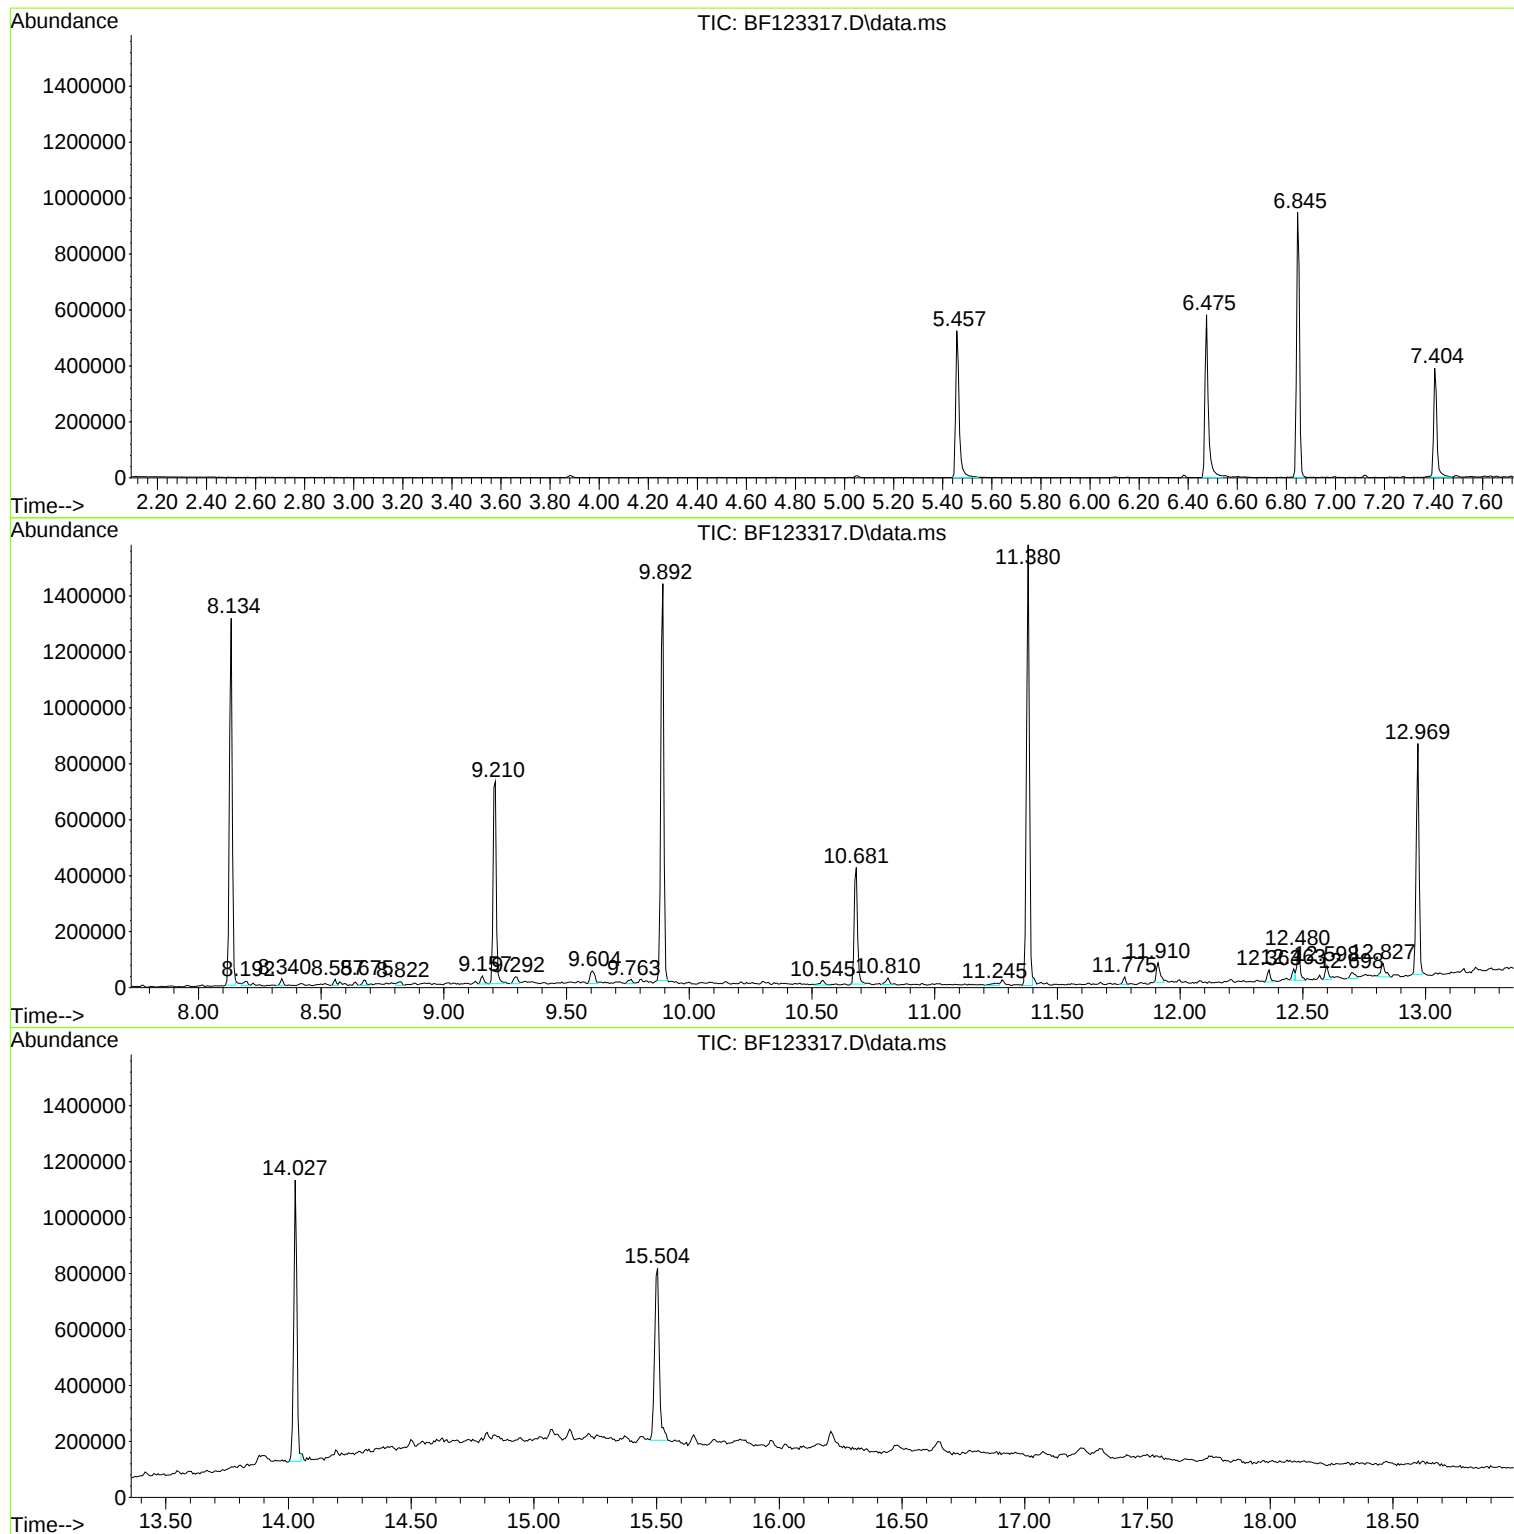

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022621\
Data File : BF123317.D
Acq On : 26 Feb 2021 23:01
Operator : JU/CG
Sample : M1491-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SA-01-022521

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022621\
Data File : BF123317.D
Acq On : 26 Feb 2021 23:01
Operator : JU/CG
Sample : M1491-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SA-01-022521

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------