


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022621\
 Data File : BF123303.D
 Acq On : 26 Feb 2021 14:28
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 16:08:53 2021

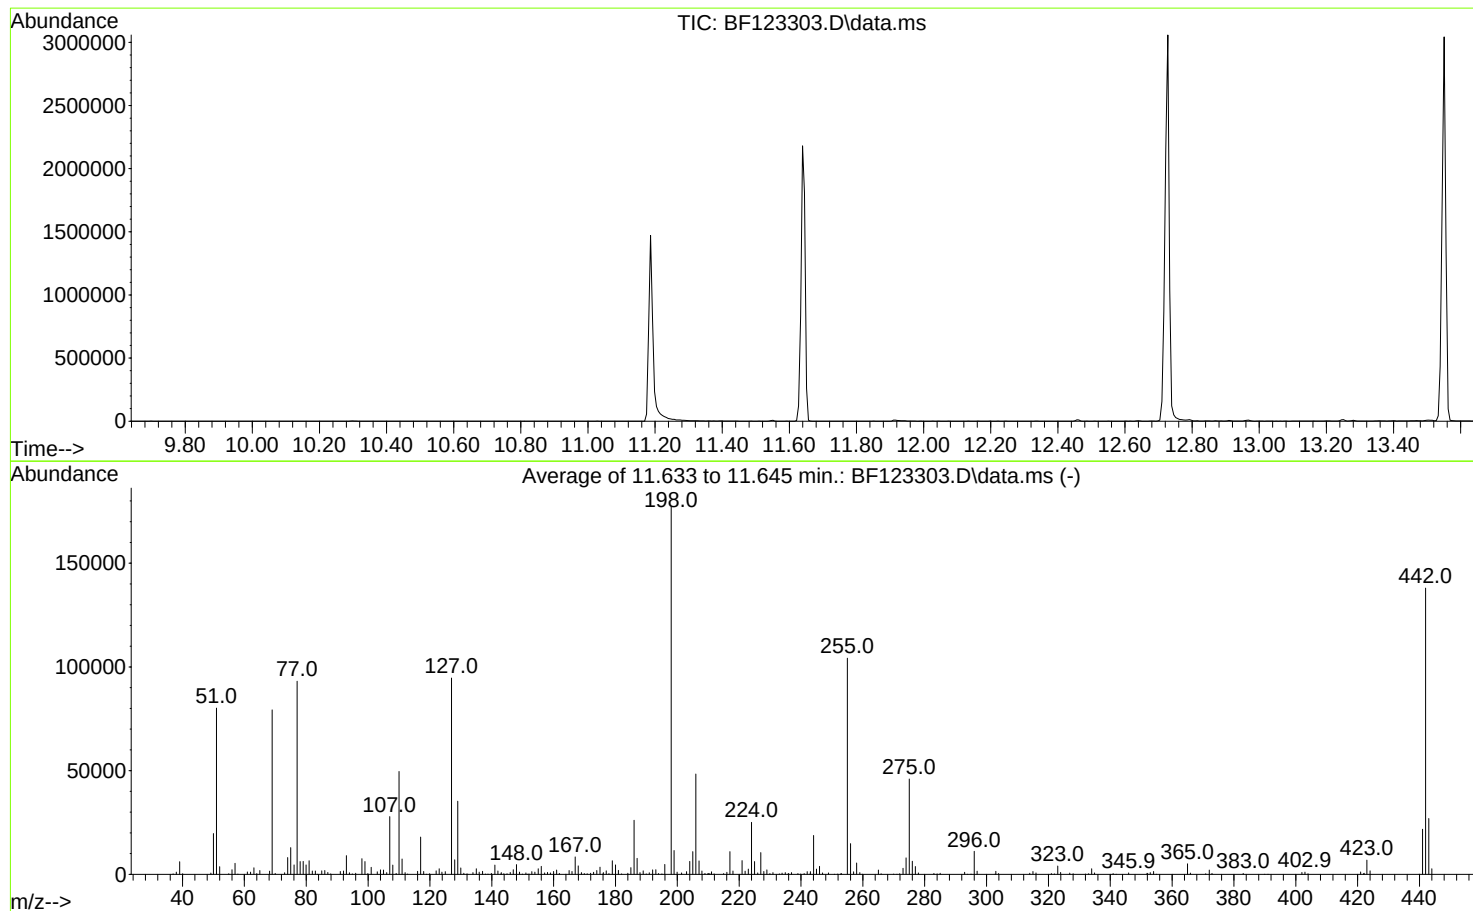

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	80136	PASS
68	69	0.00	2	2.0	1556	PASS
69	198	0.00	100	44.7	79277	PASS
70	69	0.00	2	0.6	443	PASS
127	198	10	80	53.4	94627	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	177328	PASS
199	198	5	9	6.5	11518	PASS
275	198	10	60	25.9	45957	PASS
365	198	1	100	2.9	5097	PASS
441	198	0.01	100	12.3	21725	PASS
442	442	50	100	100.0	137997	PASS
443	442	15	24	19.5	26894	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/26/2021	BNA_F	<u>BF123303.D</u>
Compound Name	Response	Retention Time
DDT	434670	13.55
DDD	2967	13.25
DDE	817	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3784	438454	0.86

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022621\
Data File : BF123303.D
Acq On : 26 Feb 2021 14:28
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 26 15:25:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

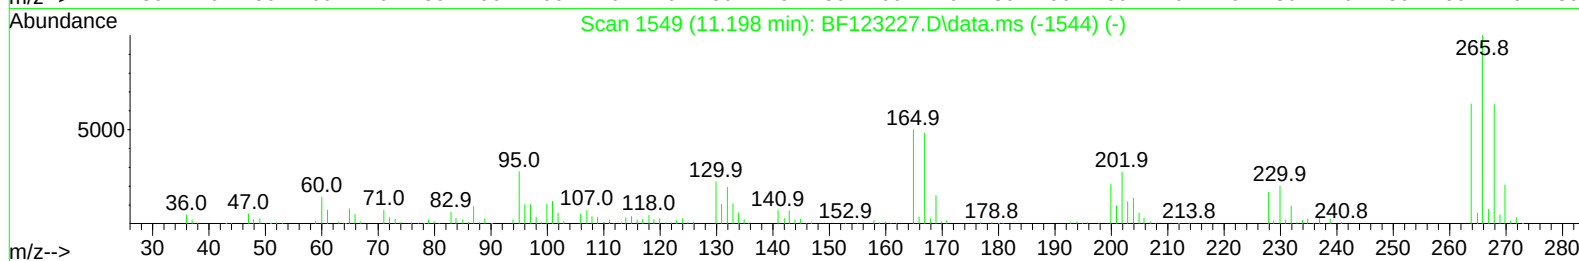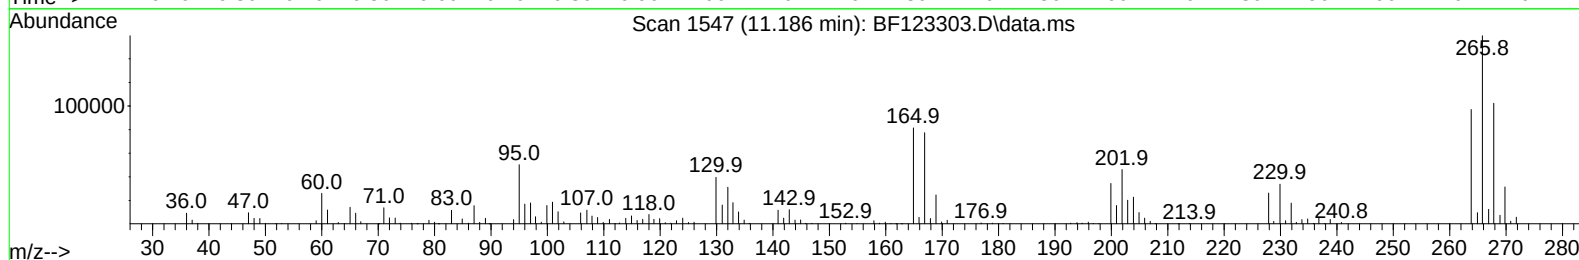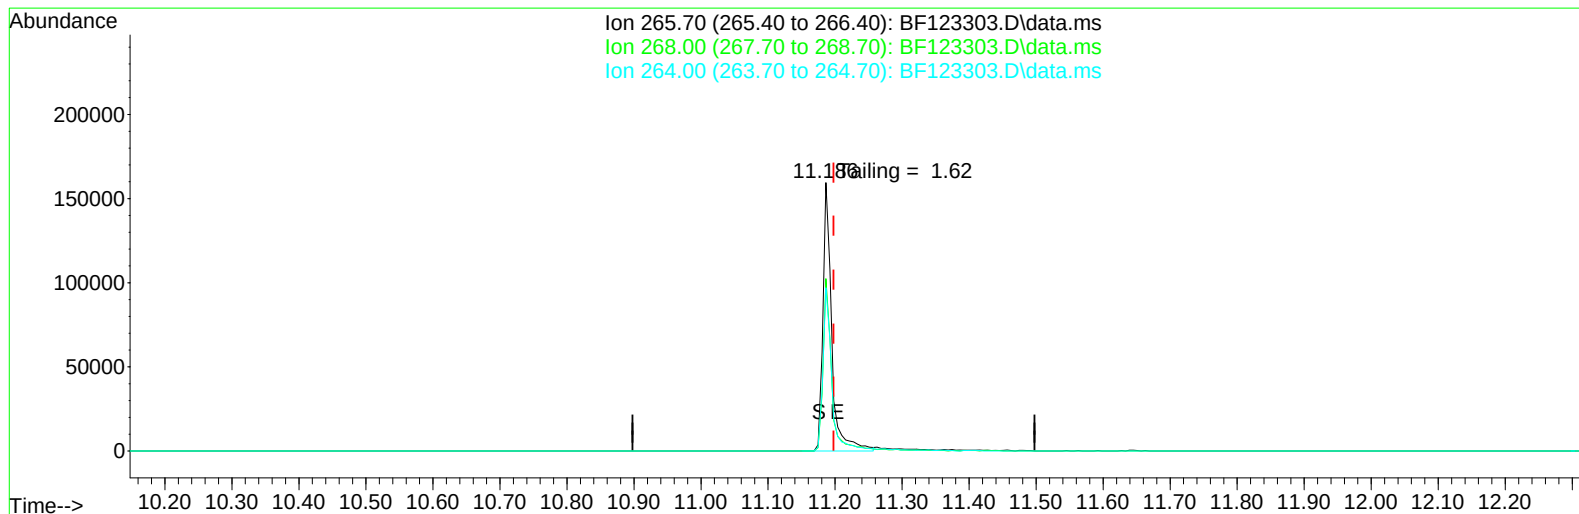

TIC: BF123303.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.012) 22908.21 ng




response 151167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.20
264.00	62.30	60.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022621\
Data File : BF123303.D
Acq On : 26 Feb 2021 14:28
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 26 15:25:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

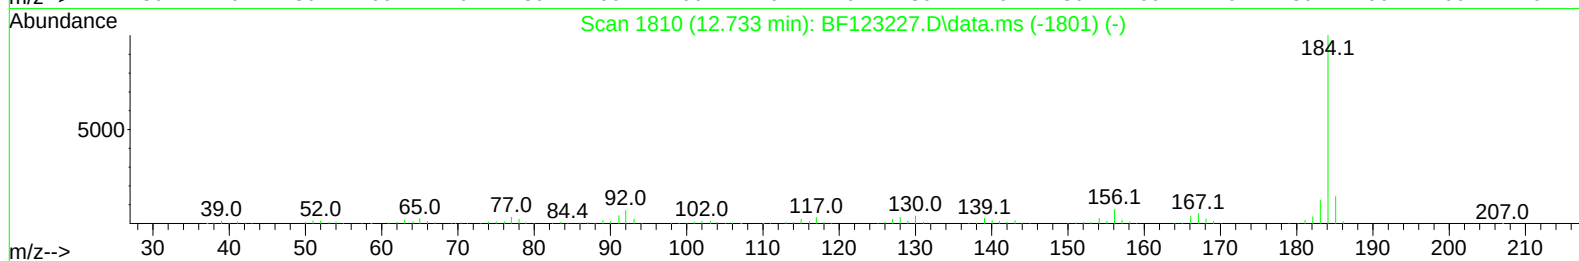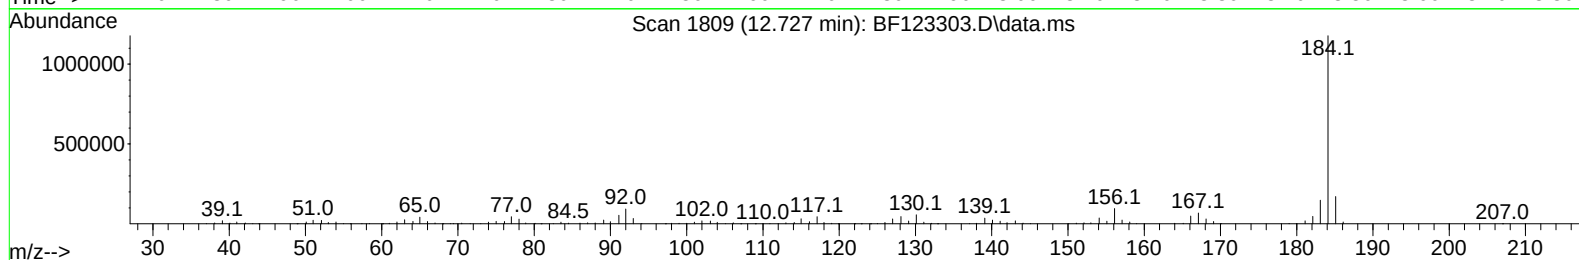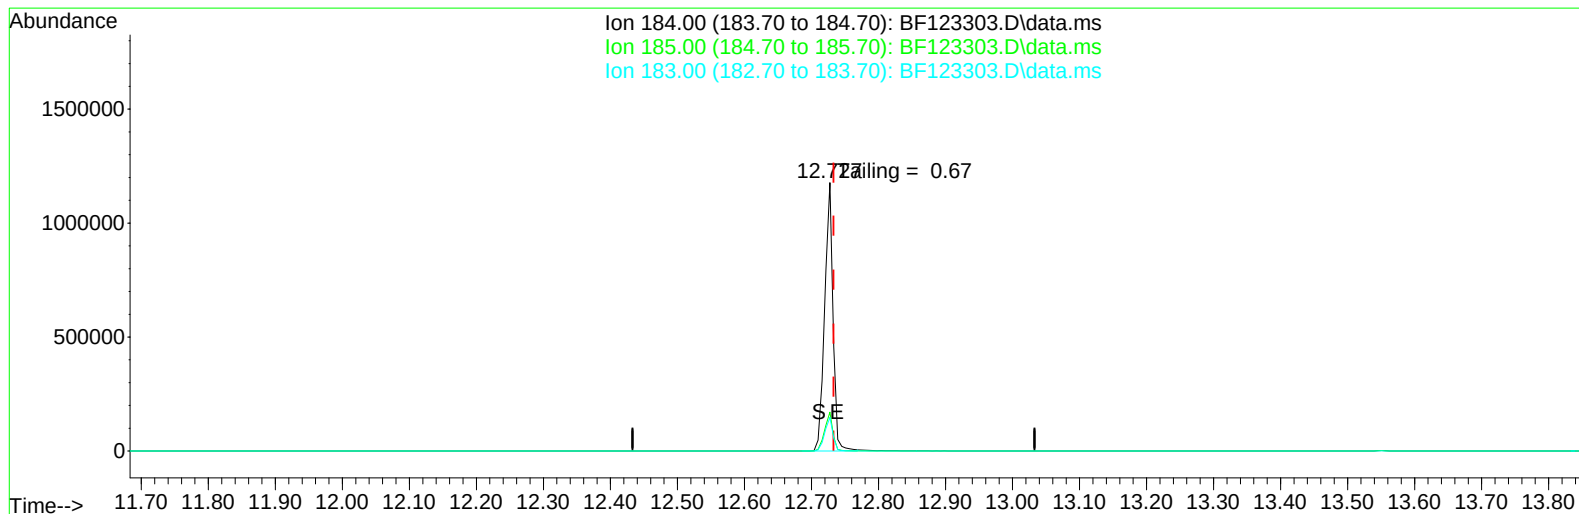

TIC: BF123303.D\data.ms

(77) Benzidine

12.727min (-0.006) 0.00 ng

response 1030495

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.50
183.00	12.10	12.54
0.00	0.00	0.00