
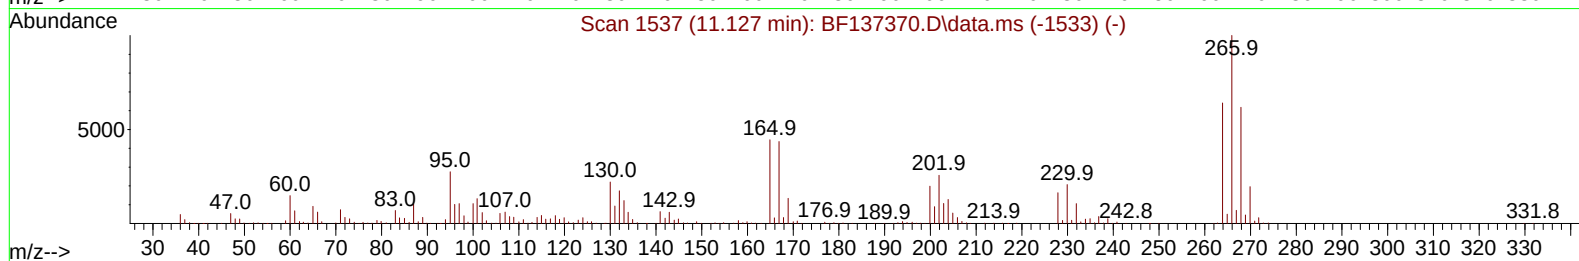
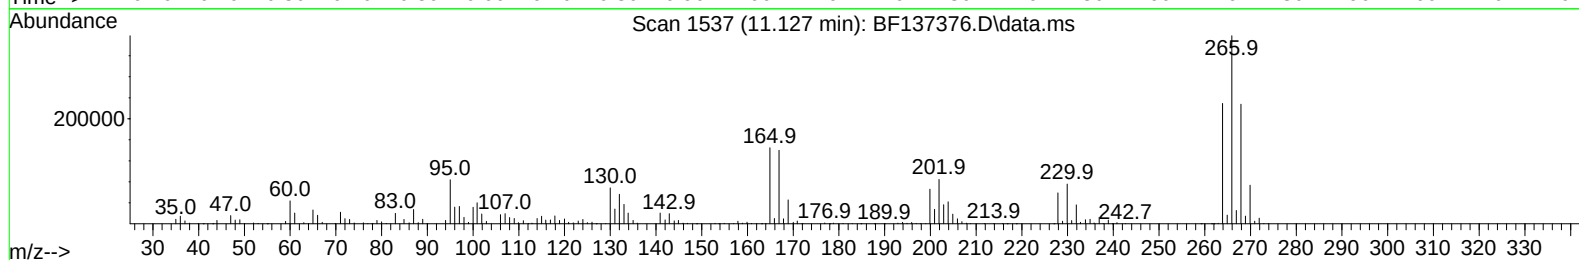


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022624\
Data File : BF137376.D
Acq On : 26 Feb 2024 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 11:20:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 04:23:49 2024
Response via : Initial Calibration

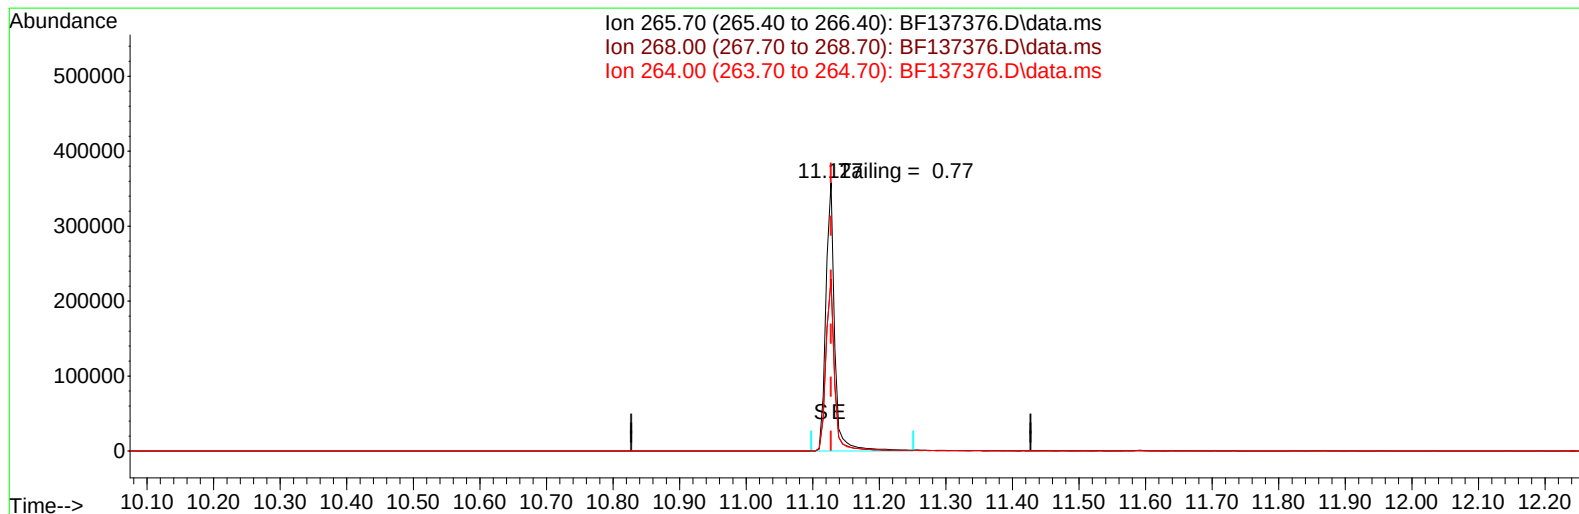

TIC: BF137376.D\data.ms

(70) Pentachlorophenol (C)




11.127min (-0.000) 208622.59 ng

response 330738

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.80	63.56
264.00	64.10	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022624\
Data File : BF137376.D
Acq On : 26 Feb 2024 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 11:20:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 04:23:49 2024
Response via : Initial Calibration

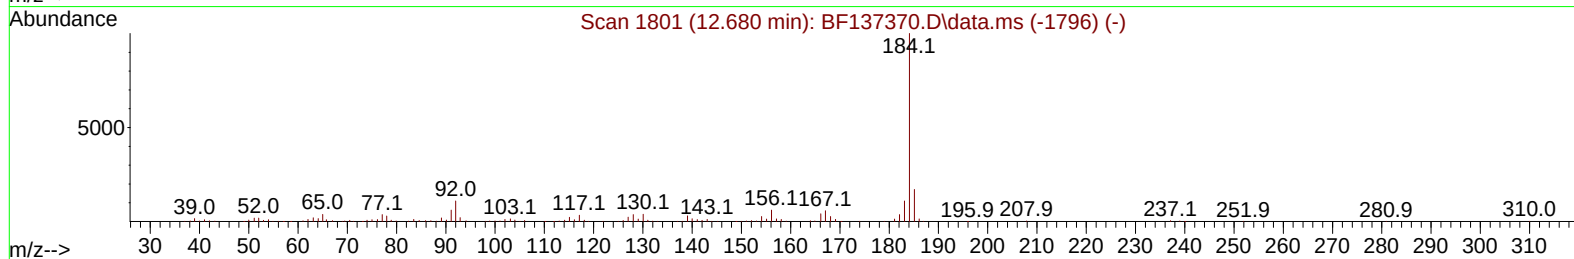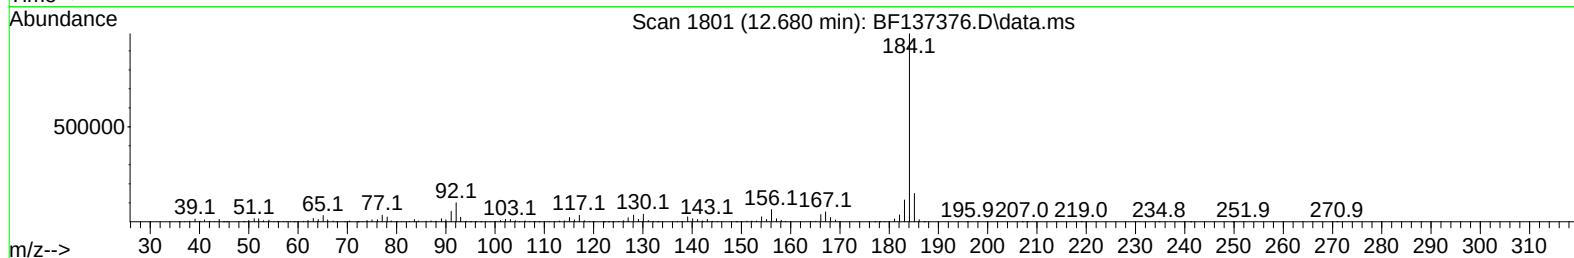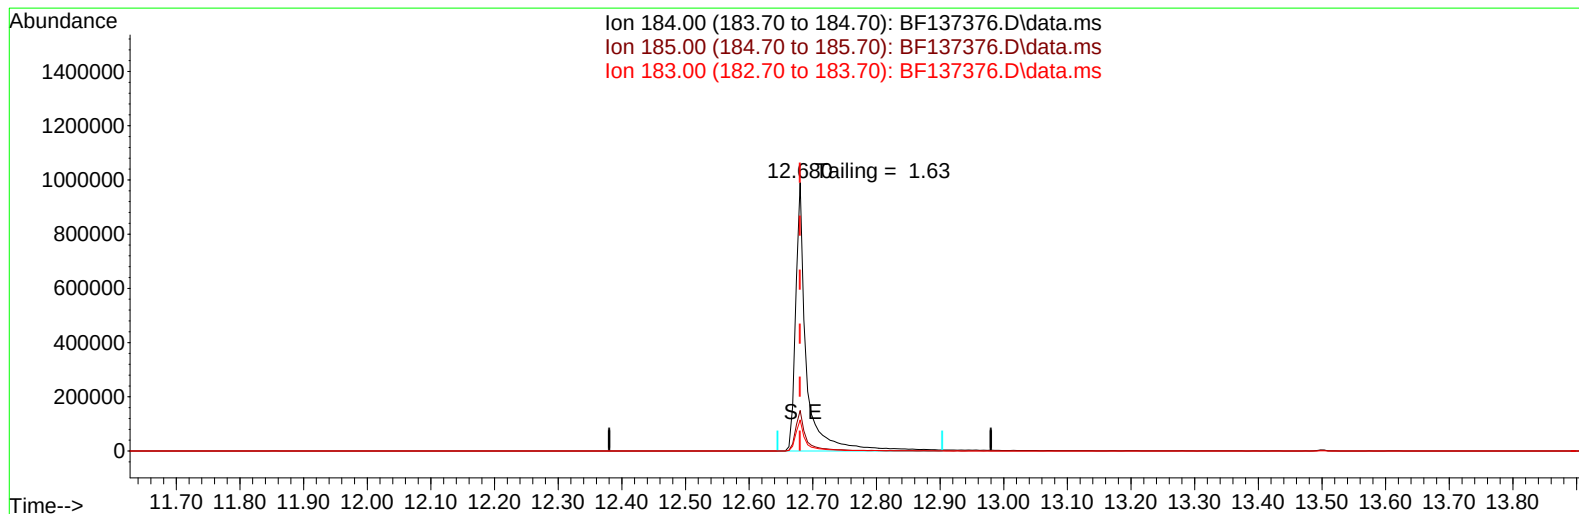

TIC: BF137376.D\data.ms

(77) Benzidine**12.680min (+ 0.000) 244781.57 ng****response 1177336**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.10	15.11
183.00	11.00	11.56
0.00	0.00	0.00