
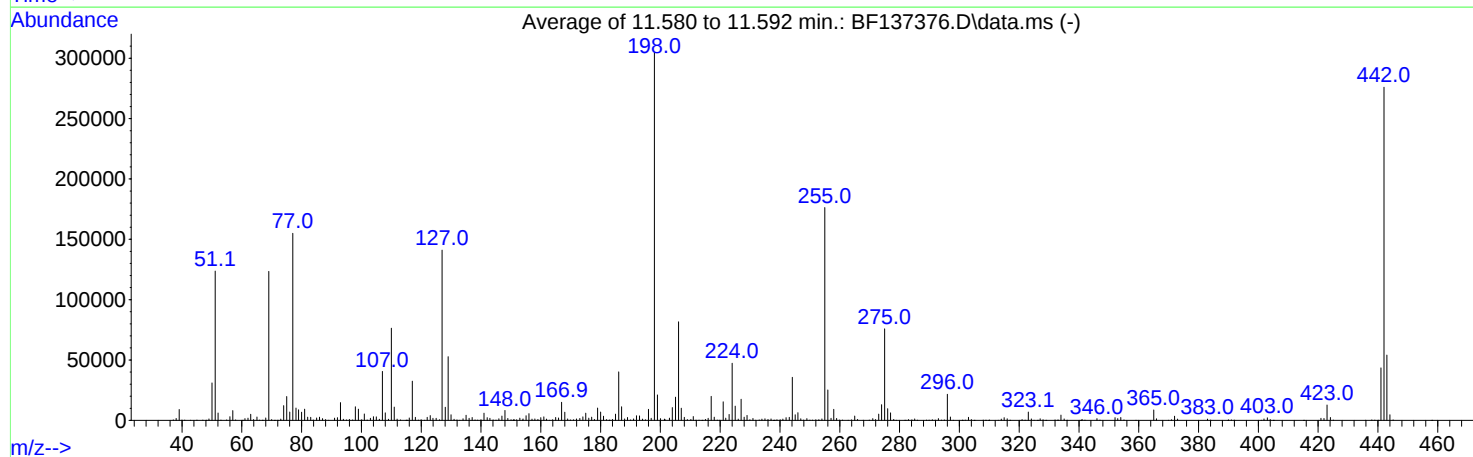


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022624\
Data File : BF137376.D
Acq On : 26 Feb 2024 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Feb 24 04:23:49 2024

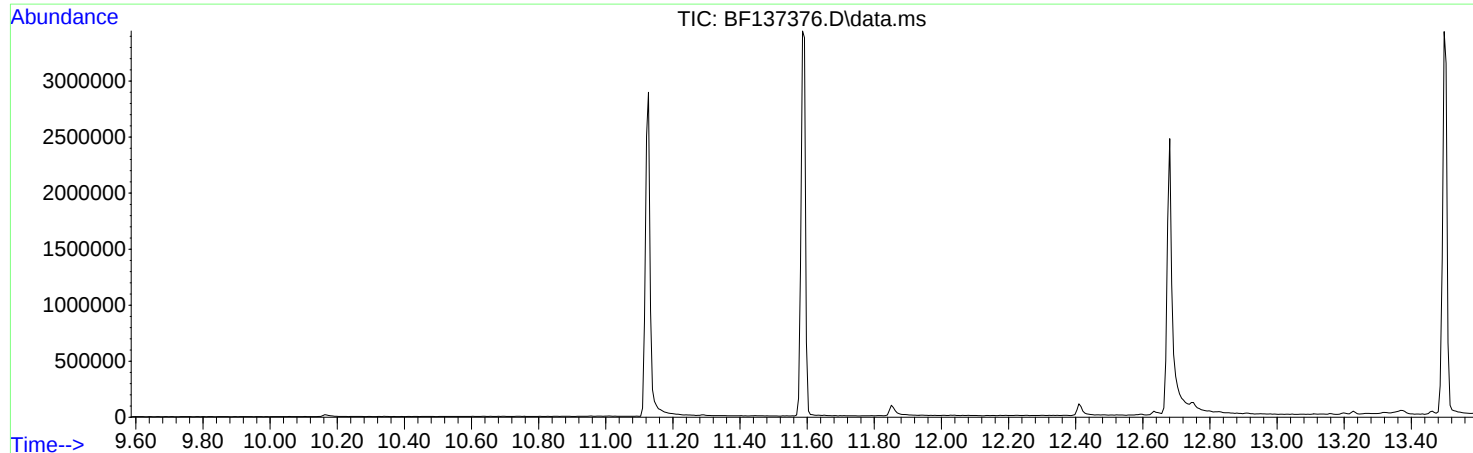




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	123661	PASS
68	69	0.00	2	1.6	1998	PASS
69	198	0.00	100	40.5	123453	PASS
70	69	0.00	2	0.6	679	PASS
127	198	10	80	46.3	141085	PASS
197	198	0.00	2	0.6	1737	PASS
198	198	100	100	100.0	304768	PASS
199	198	5	9	6.9	21129	PASS
275	198	10	60	24.9	75800	PASS
365	198	1	100	2.8	8560	PASS
441	198	0.01	100	14.3	43443	PASS
442	442	50	100	100.0	276037	PASS
443	442	15	24	19.6	54135	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022624\
Data File : BF137376.D
Acq On : 26 Feb 2024 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 26 11:20:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 04:23:49 2024
Response via : Initial Calibration

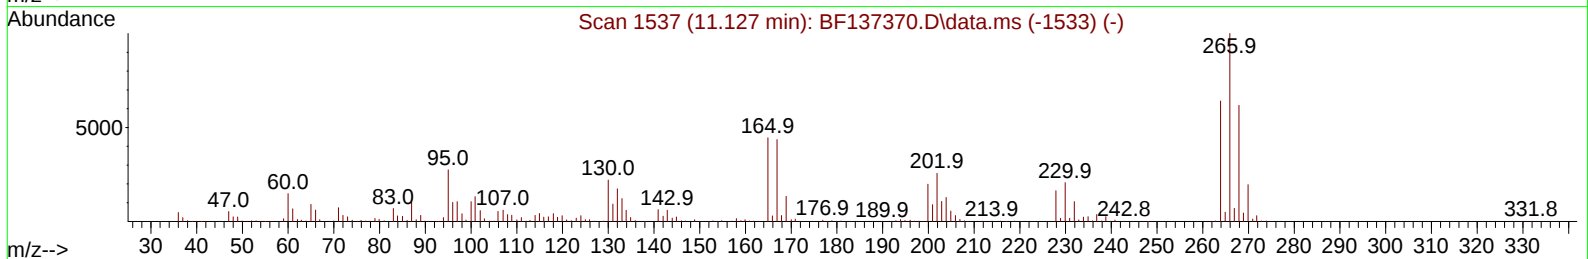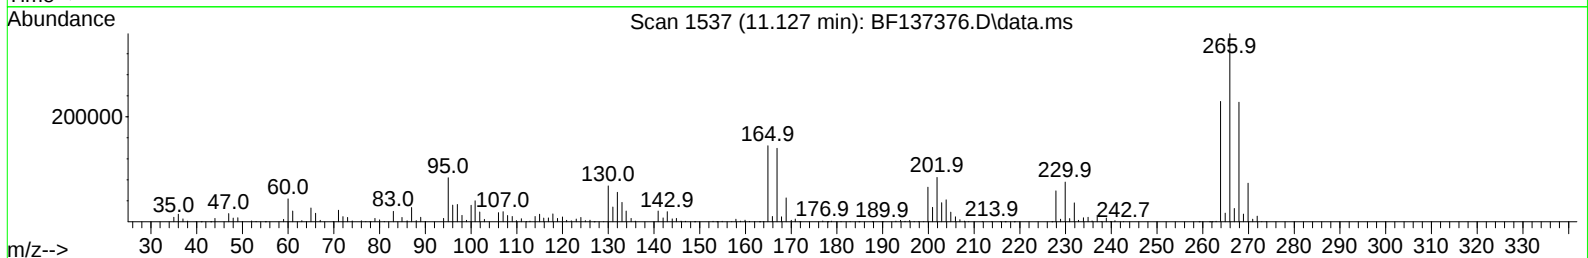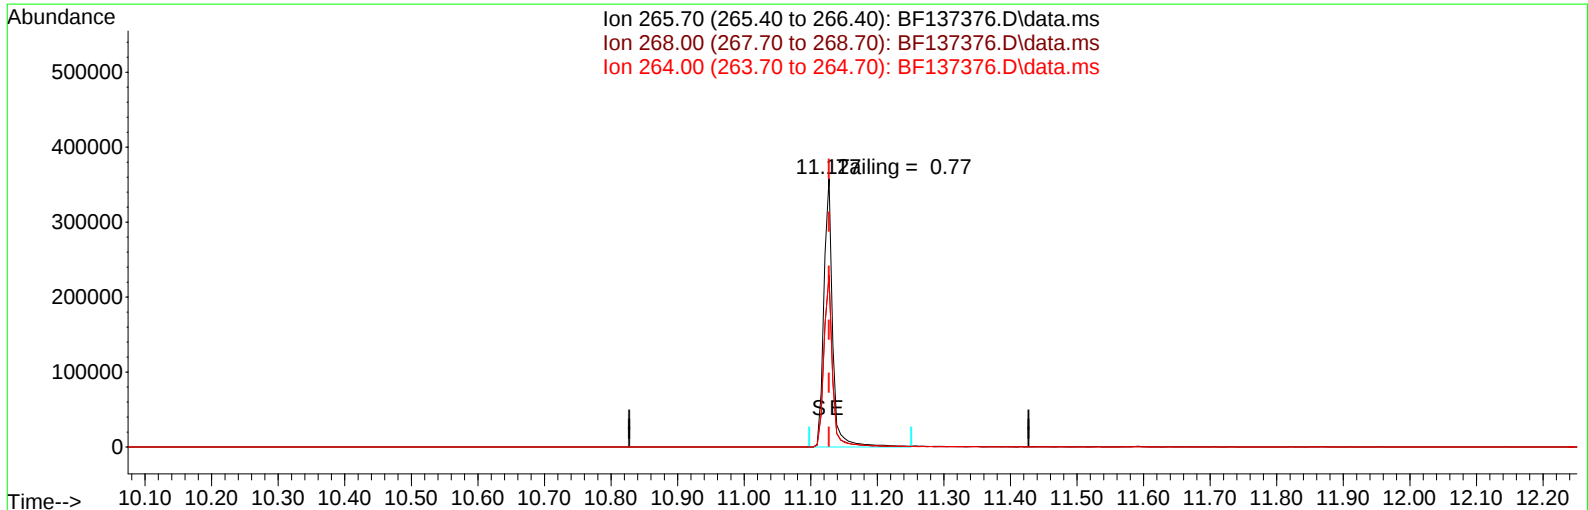

TIC: BF137376.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 208622.59 ng




response 330738

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.80	63.56
264.00	64.10	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022624\
Data File : BF137376.D
Acq On : 26 Feb 2024 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 26 11:20:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 04:23:49 2024
Response via : Initial Calibration

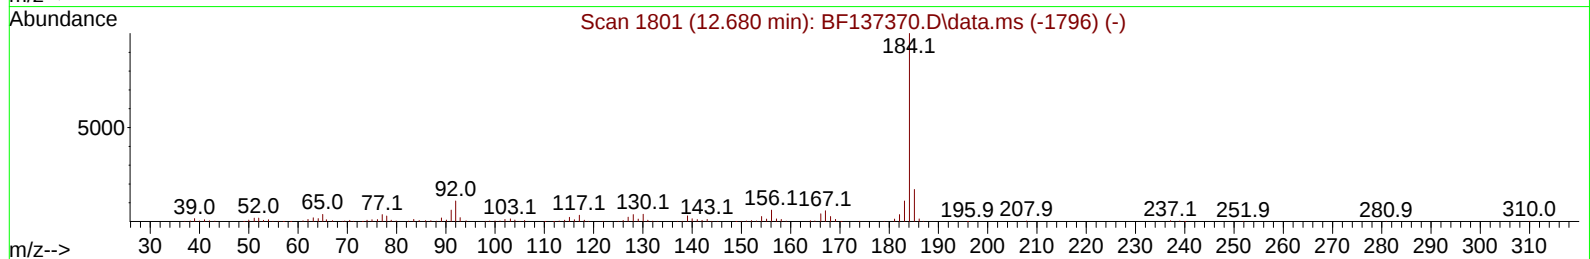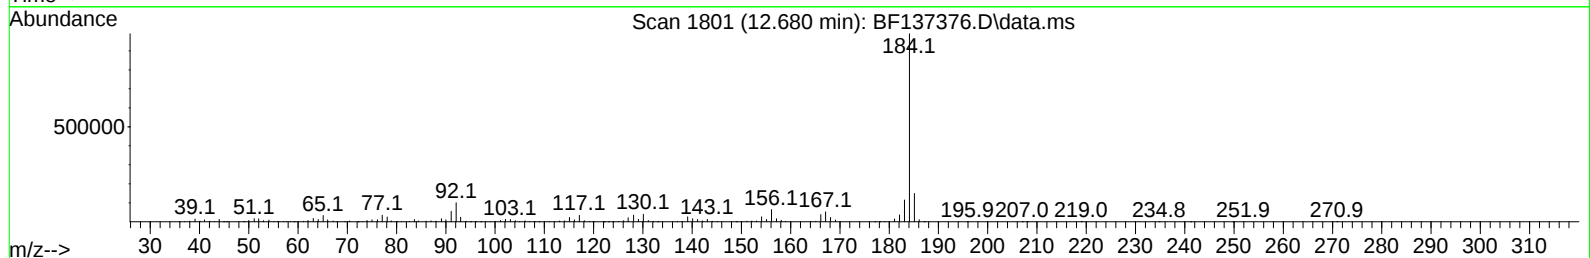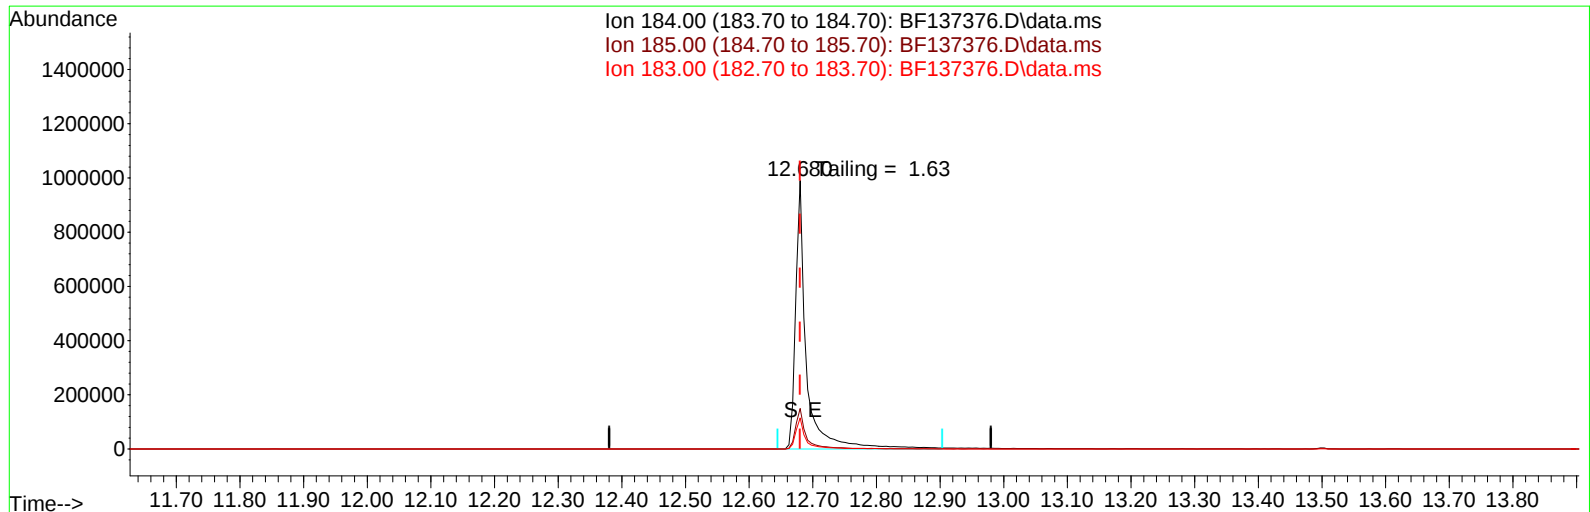

TIC: BF137376.D\data.ms

(77) Benzidine

12.680min (+ 0.000) 244781.57 ng

response 1177336

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.10	15.11
183.00	11.00	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/26/2024	BNA_F	<u>BF137376.D</u>
Compound Name	Response	Retention Time
DDT	489594	13.504
DDD	6174	13.227
DDE	415	12.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6589	496183	1.33

Instrument :
BNA_F
ClientSampleId :
DFTPP