

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
 Data File : BF141778.D
 Acq On : 26 Feb 2025 12:56
 Operator : RC/JU
 Sample : PB166870BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166870BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.834	290	296	311	rVB	29790	55622	1.63%	0.299%
2	5.410	559	564	602	rBV	1710762	2477571	72.73%	13.312%
3	6.428	731	737	759	rBV	1673664	2440394	71.64%	13.113%
4	6.781	792	797	813	rVB	376531	473912	13.91%	2.546%
5	7.345	887	893	932	rBV	1142123	1644721	48.28%	8.837%
6	8.063	1009	1015	1036	rBV	432745	628799	18.46%	3.379%
7	9.139	1192	1198	1223	rBV	2287922	3136602	92.07%	16.853%
8	9.816	1307	1313	1330	rBV	512365	729671	21.42%	3.921%
9	10.610	1442	1448	1476	rBV	1233617	1836544	53.91%	9.868%
10	11.304	1560	1566	1591	rBV	519222	753051	22.11%	4.046%
11	12.886	1829	1835	1851	rBV	2517954	3406630	100.00%	18.304%
12	13.945	2009	2015	2030	rBV	375328	579002	17.00%	3.111%
13	15.392	2255	2261	2280	rBV	239629	448595	13.17%	2.410%




Sum of corrected areas: 18611114

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141778.D
Acq On : 26 Feb 2025 12:56
Operator : RC/JU
Sample : PB166870BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166870BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

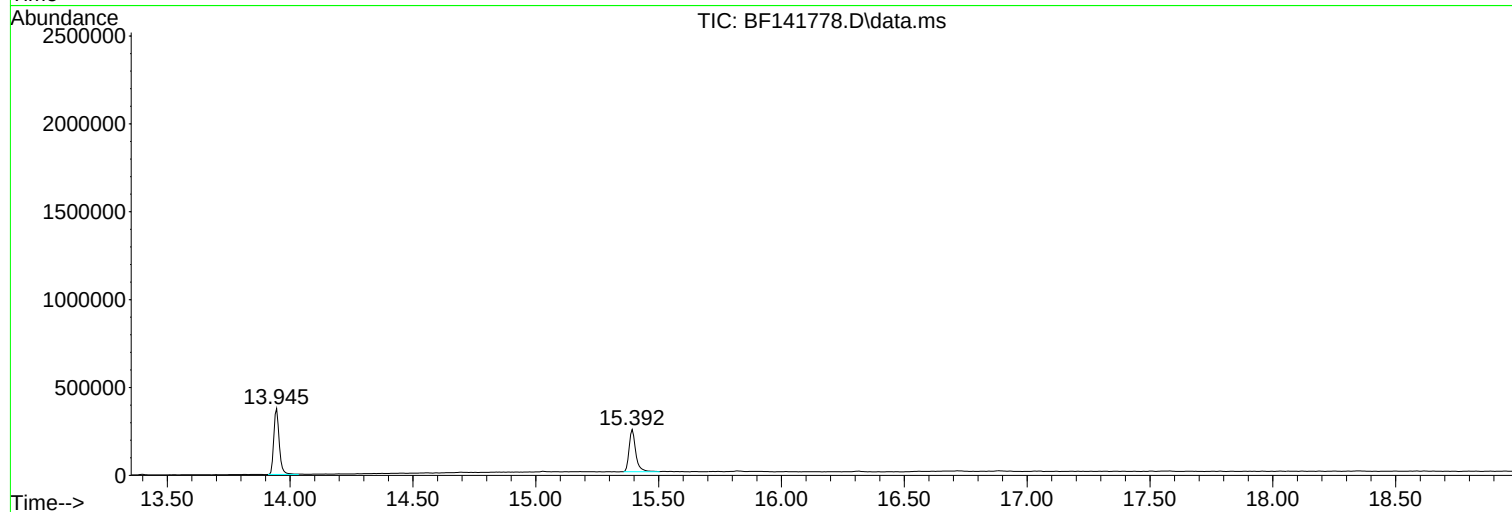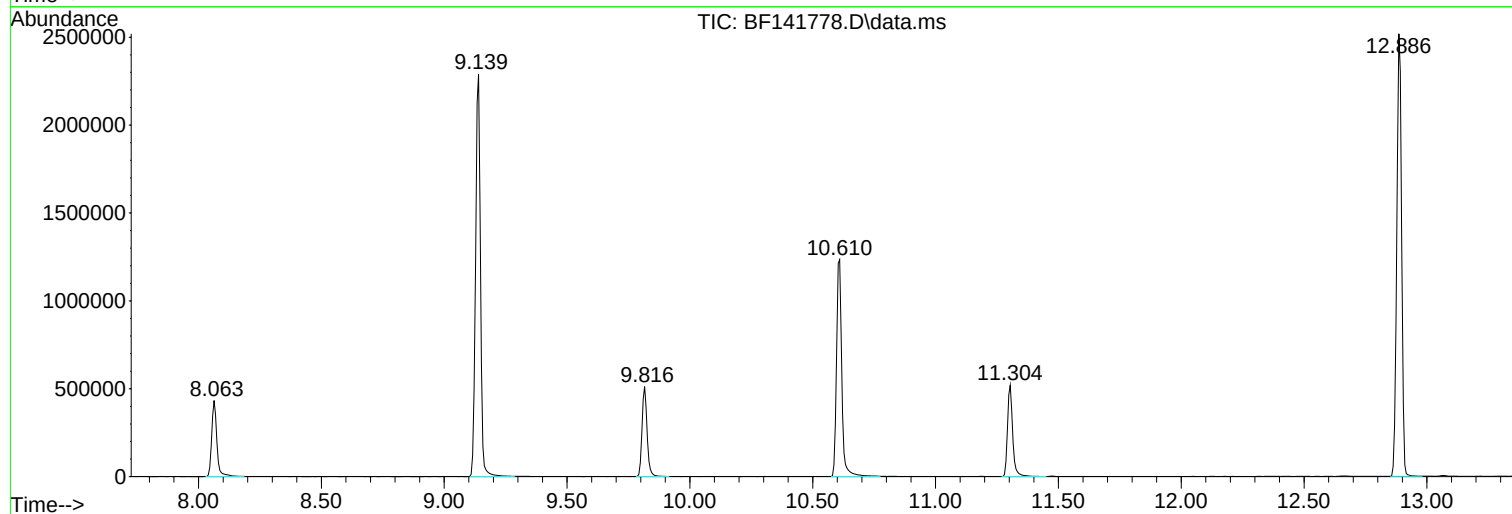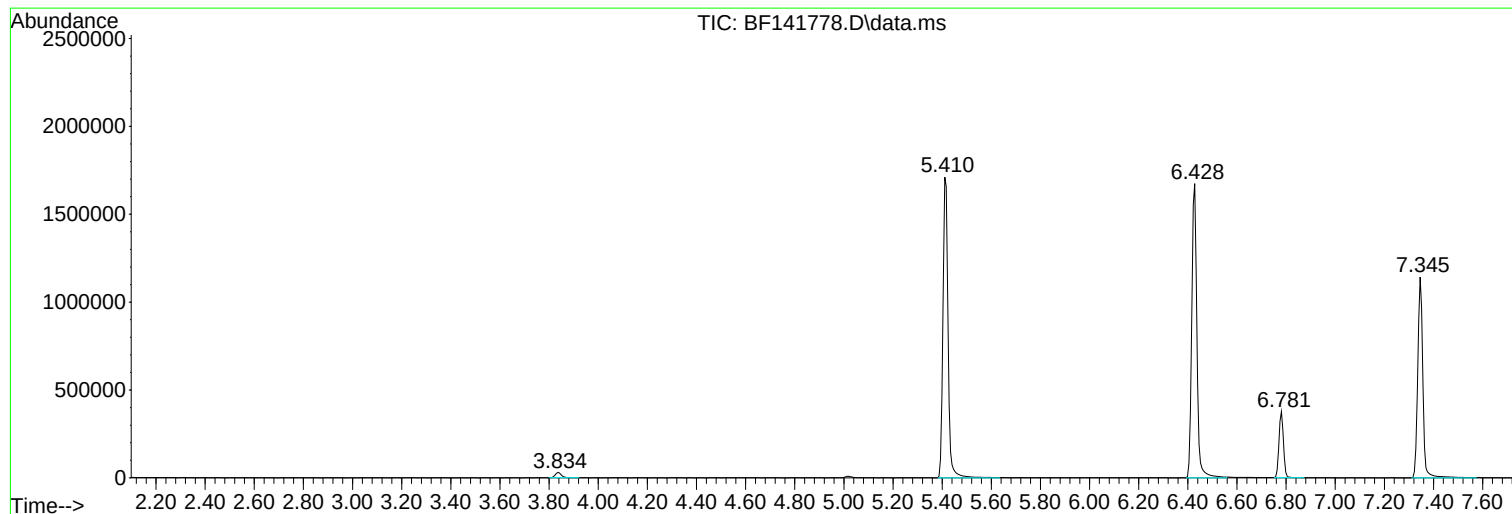

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141778.D
Acq On : 26 Feb 2025 12:56
Operator : RC/JU
Sample : PB166870BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166870BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141778.D
Acq On : 26 Feb 2025 12:56
Operator : RC/JU
Sample : PB166870BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166870BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------