


Data Path : Z:\HPCHEM1\BNA_F\Data\BF022715\
 Data File : BF077502.D
 Acq On : 27 Feb 2015 12:09
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 27 07:02:57 2015

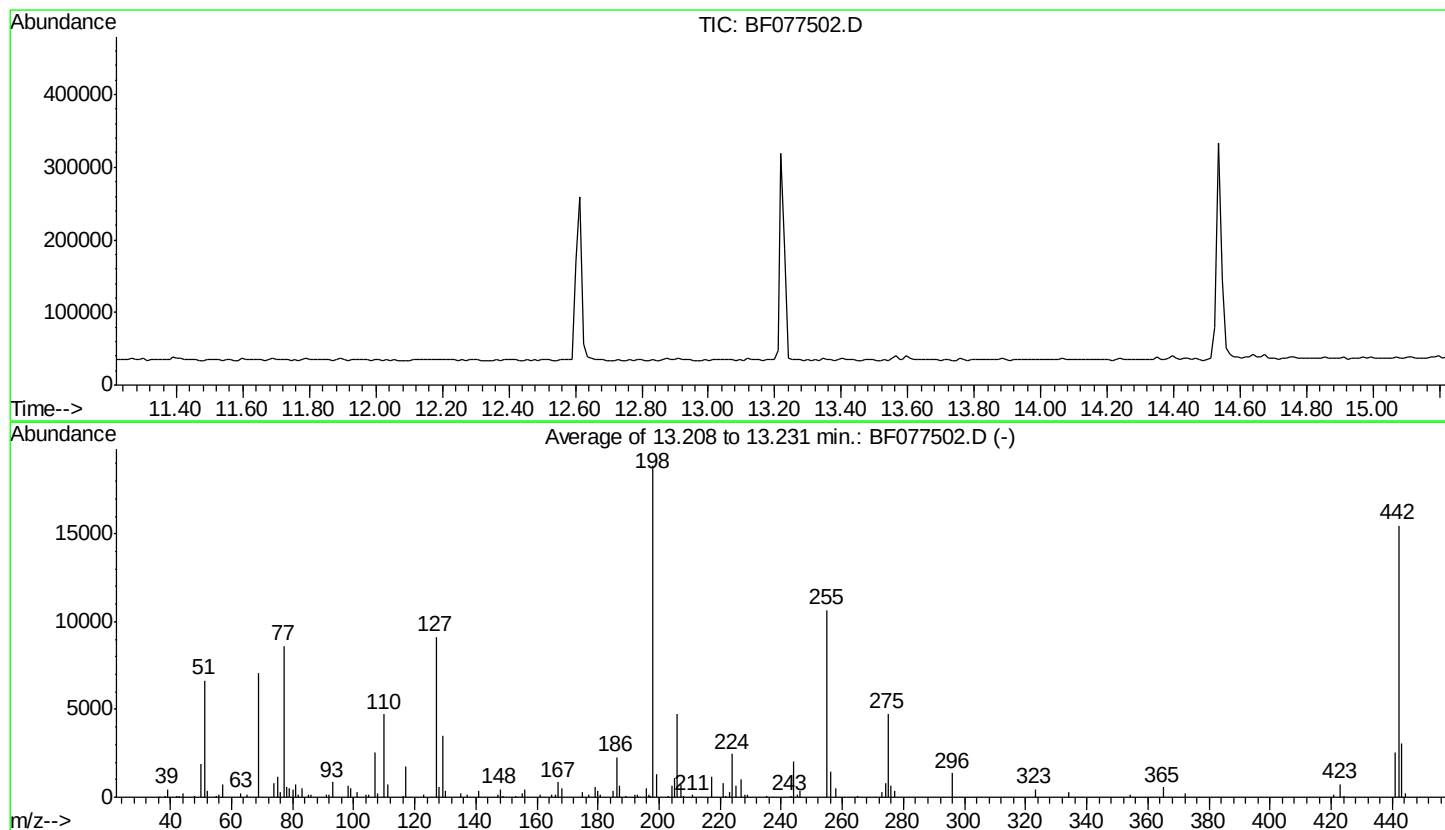

AutoFind: Scans 1078, 1079, 1080; Background Corrected with Scan 1075

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	6668	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.3	7039	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	9134	PASS
197	198	0.00	2	0.6	117	PASS
198	198	100	100	100.0	18883	PASS
199	198	5	9	6.8	1287	PASS
275	198	10	60	25.3	4769	PASS
365	198	1	100	3.0	561	PASS
441	442	0.01	24	16.4	2543	PASS
442	198	50	100	81.9	15464	PASS
443	442	15	24	19.8	3065	PASS