
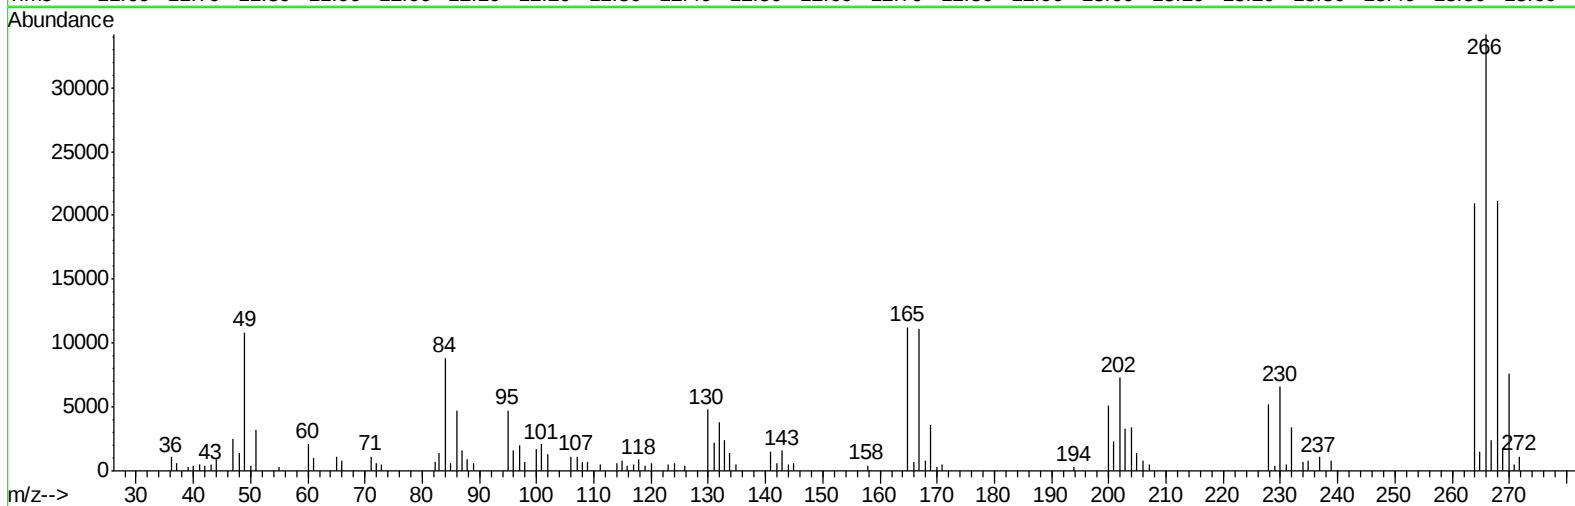


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022715\
Data File : BF077502.D
Acq On : 27 Feb 2015 12:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 05:39:56 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 27 22:28:54 2015
Response via : Initial Calibration

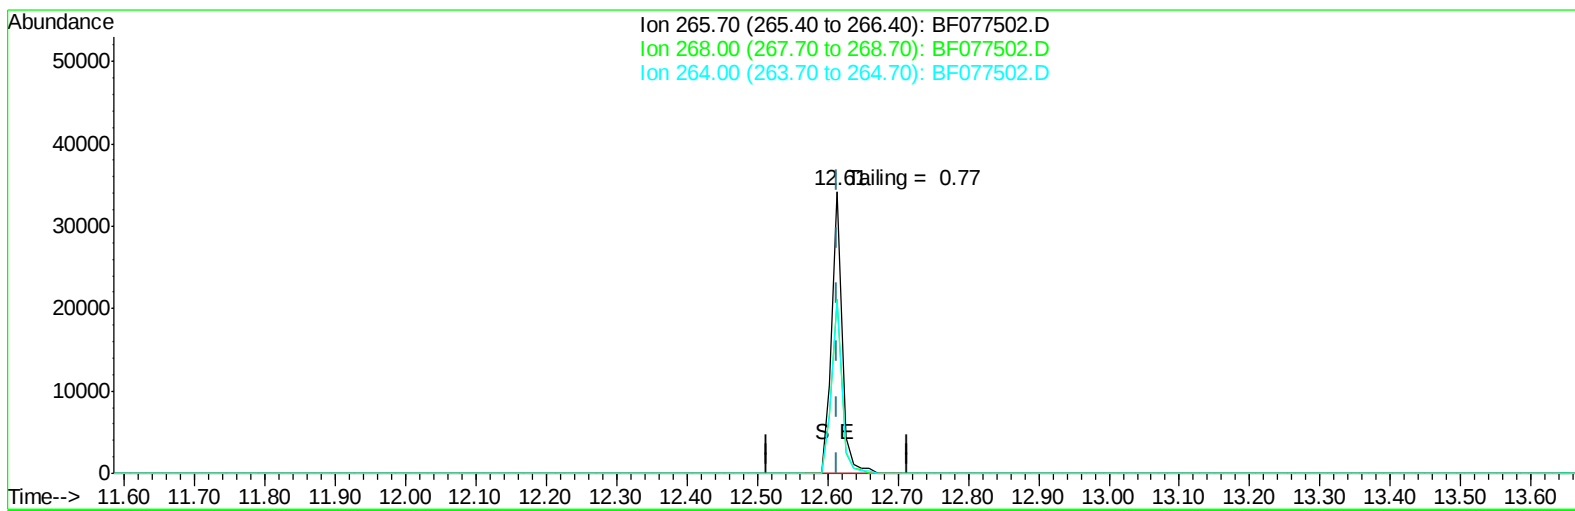

TIC: BF077502.D

(69) Pentachlorophenol (C)



12.614min (-0.001) 0.00ng

response 35382

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	61.96
264.00	63.40	61.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022715\
Data File : BF077502.D
Acq On : 27 Feb 2015 12:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 05:39:56 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 27 22:28:54 2015
Response via : Initial Calibration

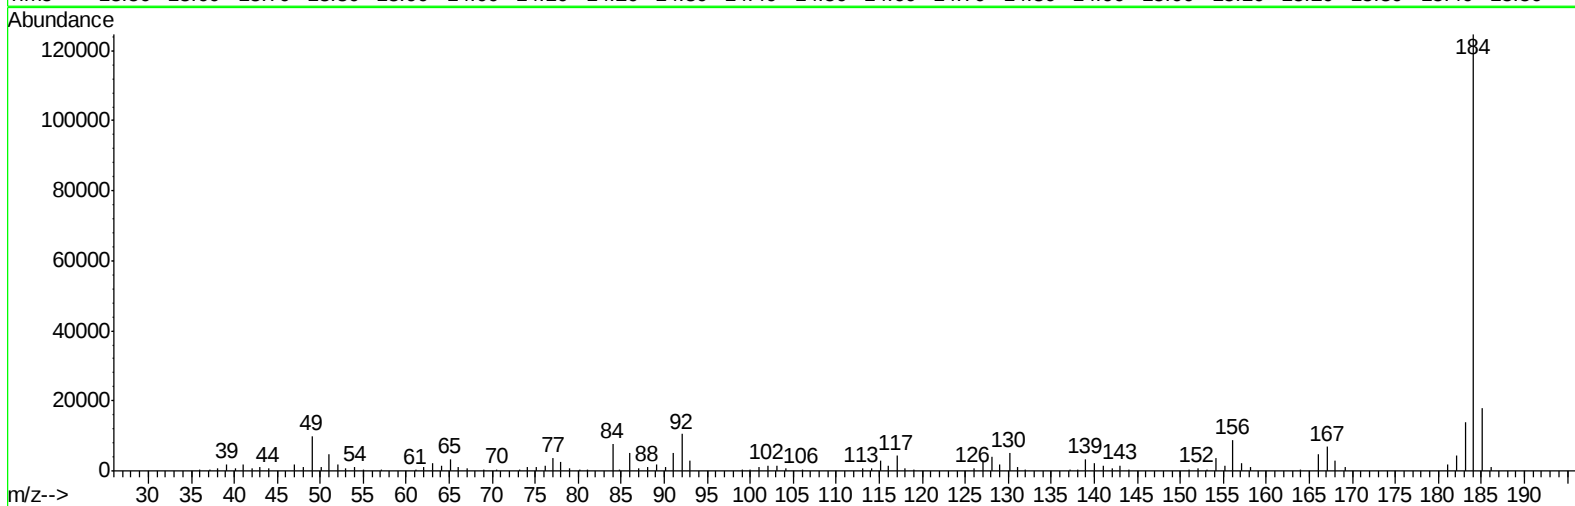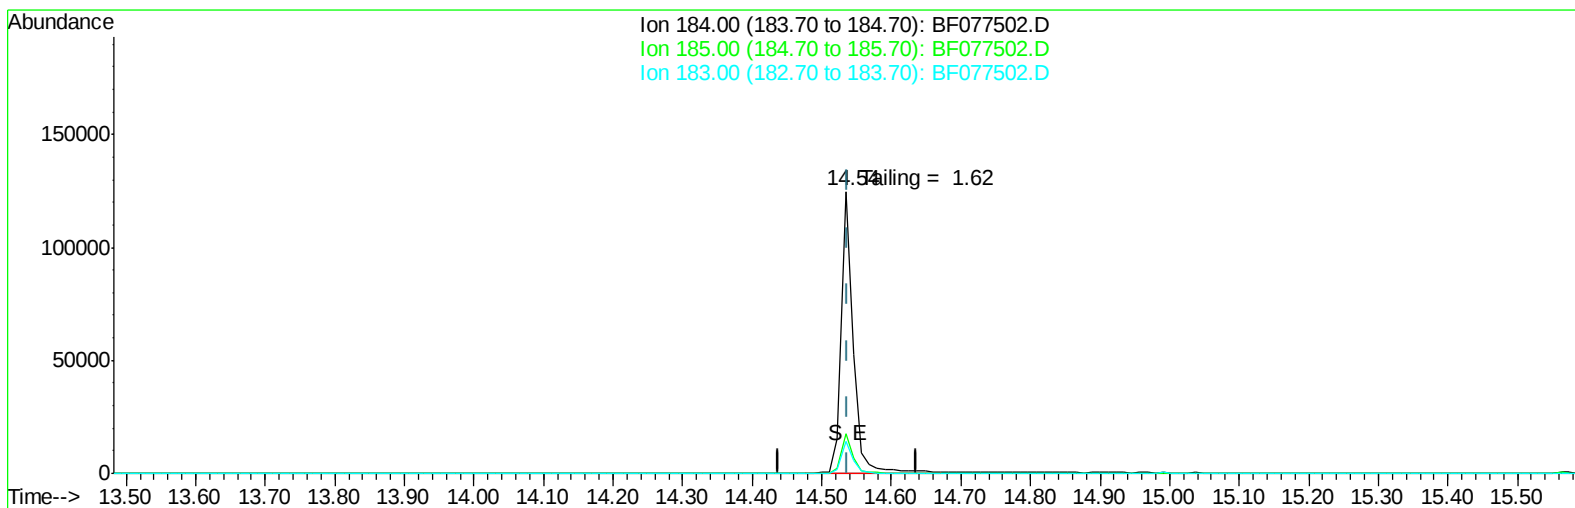

TIC: BF077502.D

(76) Benzidine

14.538min (+0.001) 0.00ng

response 144579

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.24
183.00	11.60	11.25
0.00	0.00	0.00