
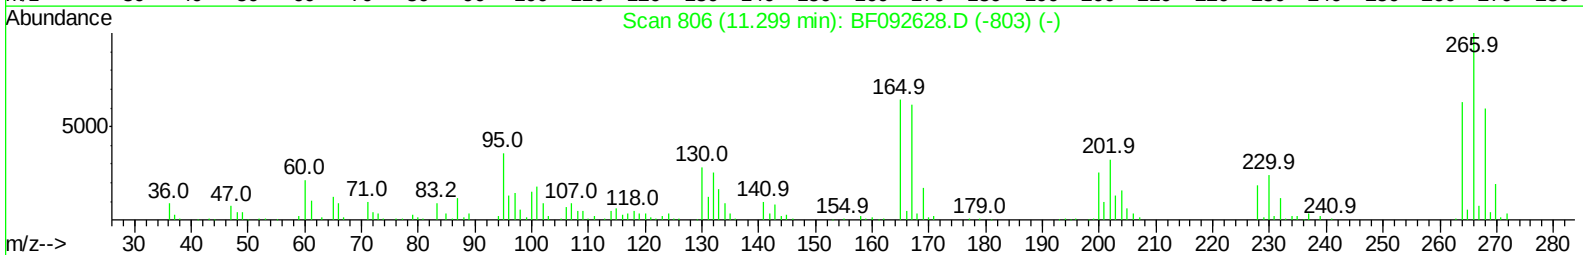
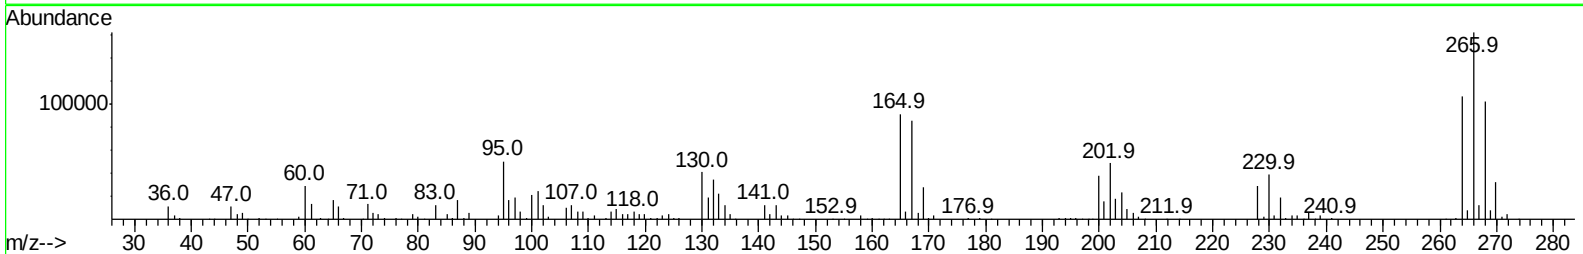


Data Path : Z:\HPCHEM1\BNA F\DATA\BF022717\
Data File : BF093197.D
Acq On : 27 Feb 2017 9:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 18:13:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

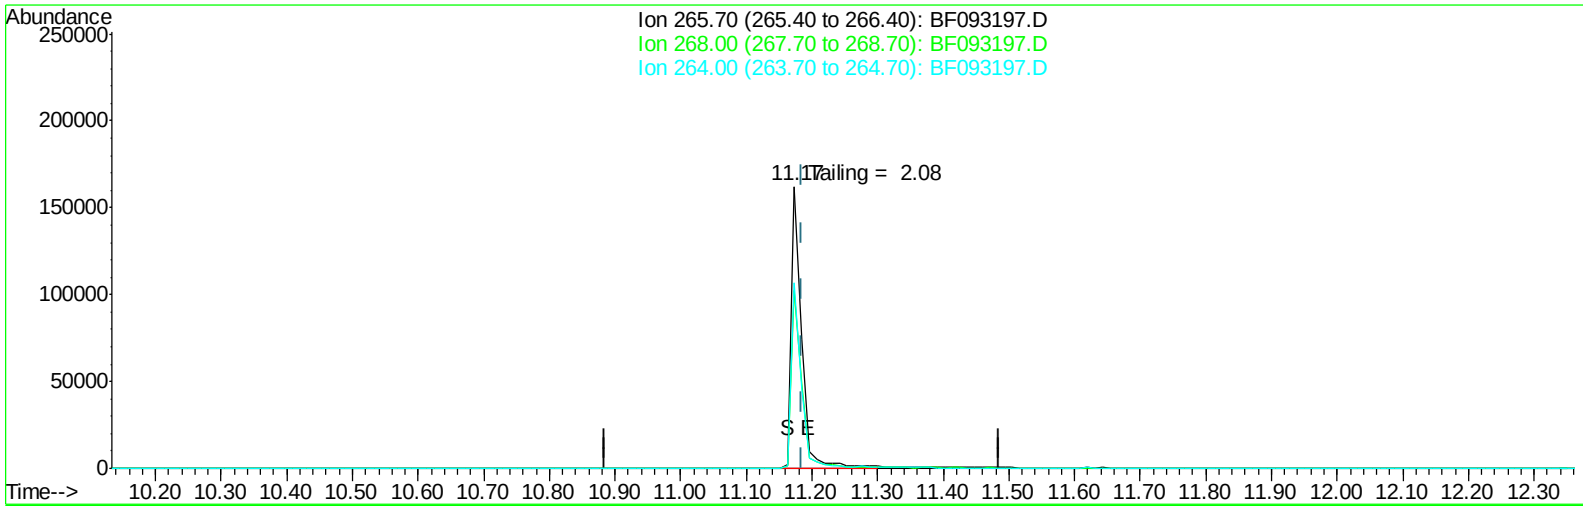

TIC: BF093197.D

(69) Pentachlorophenol (C)




11.173min (-0.011) 43193.29ng

response 187681

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.24
264.00	62.90	66.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022717\
Data File : BF093197.D
Acq On : 27 Feb 2017 9:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 18:13:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

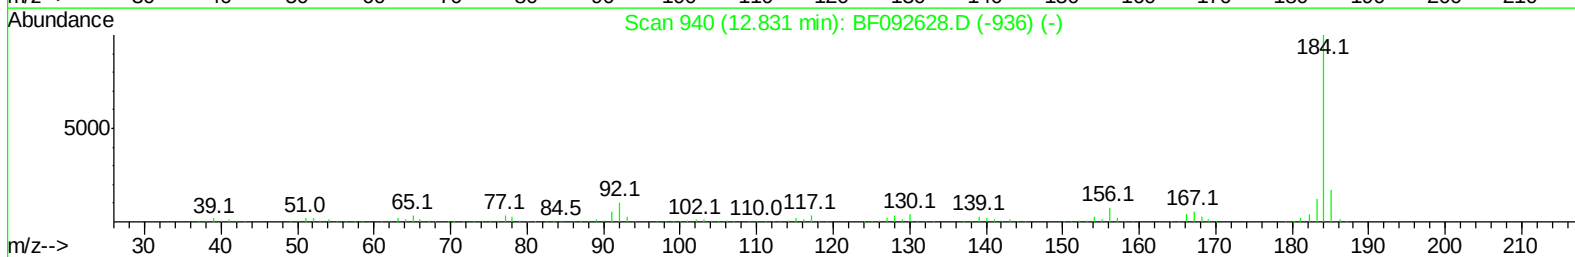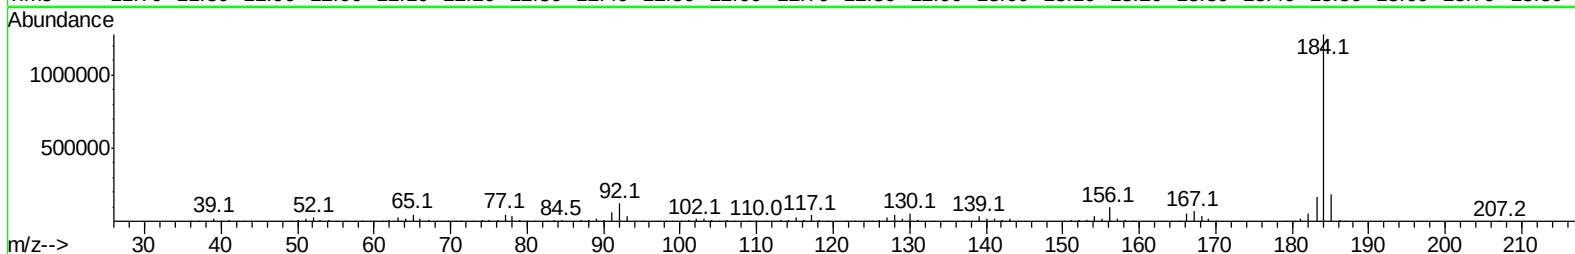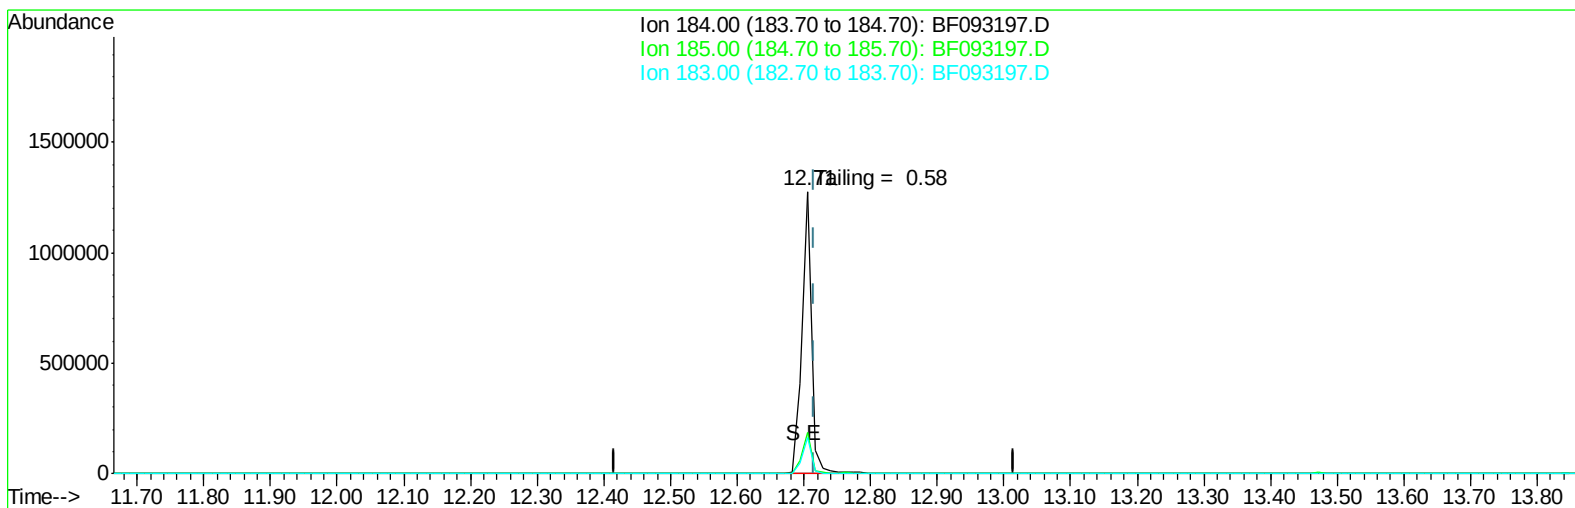

TIC: BF093197.D

(76) Benzidine

12.705min (-0.011) 0.00ng

response 1280874

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.36
183.00	11.50	12.92
0.00	0.00	0.00