

Data File : BF093212.D

Acq On : 27 Feb 2017 18:44

Operator : SJ/MA

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Feb 28 06:15:24 2017

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 28 00:51:02 2017

Response via : Initial Calibration

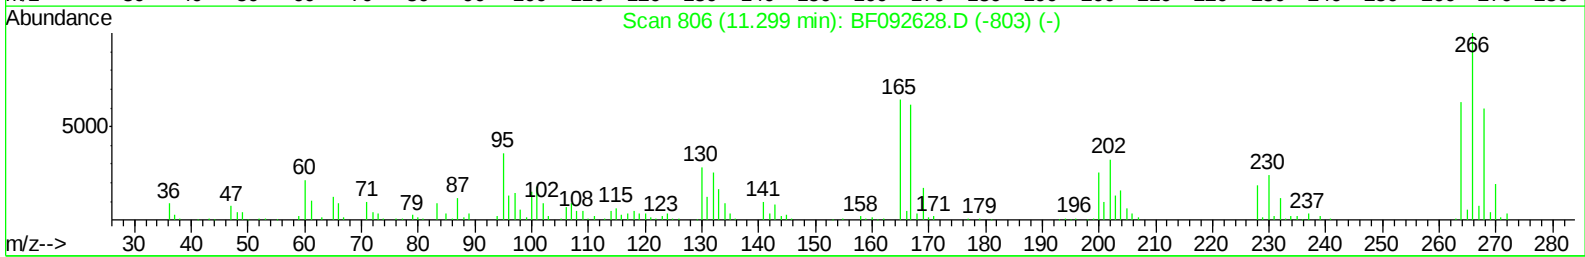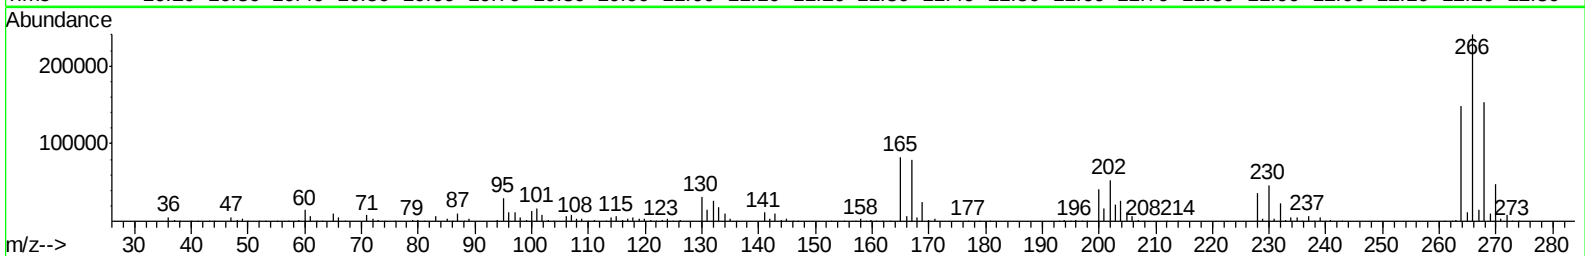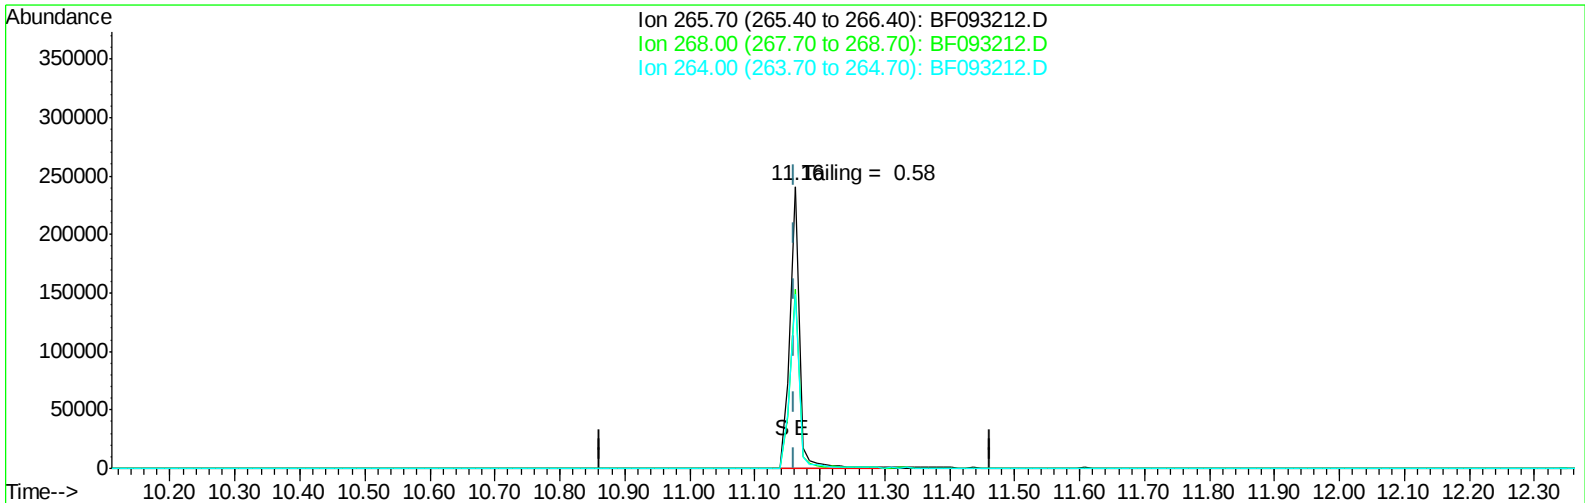

TIC: BF093212.D

(69) Pentachlorophenol (C)




11.162min (-0.000) 0.00ng

response 247353

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.64
264.00	62.90	61.94
0.00	0.00	0.00

Data File : BF093212.D
Acq On : 27 Feb 2017 18:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 06:15:24 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 00:51:02 2017
Response via : Initial Calibration

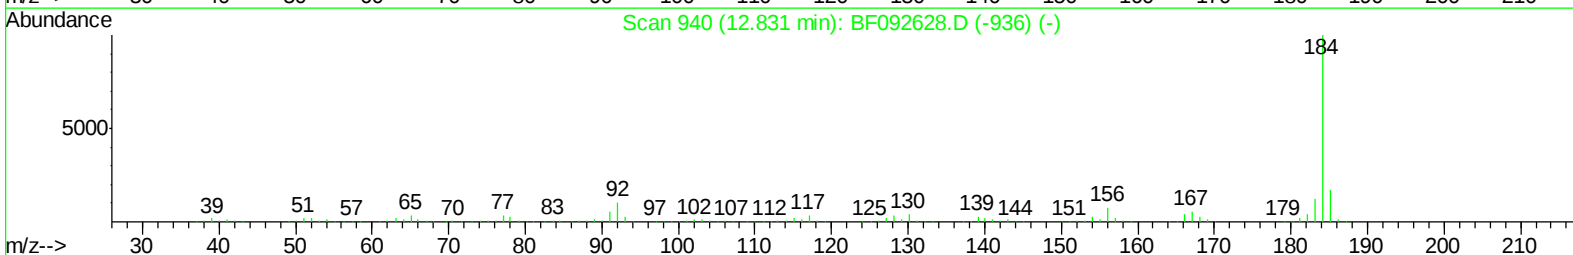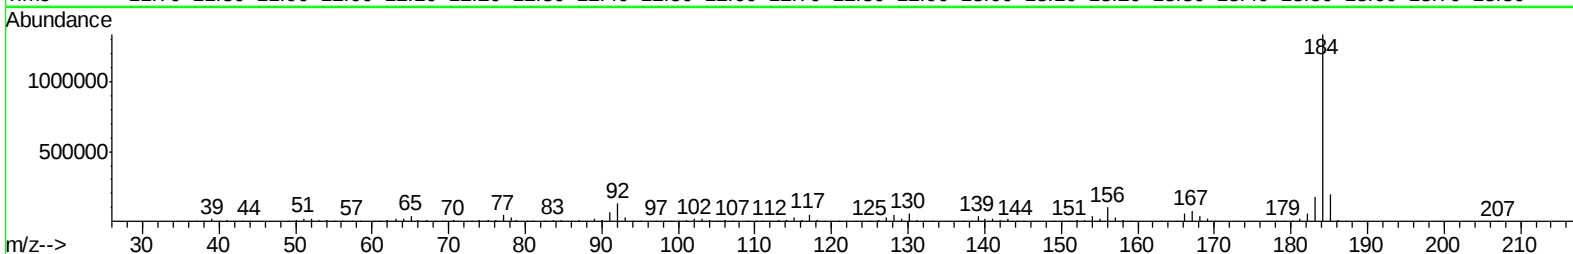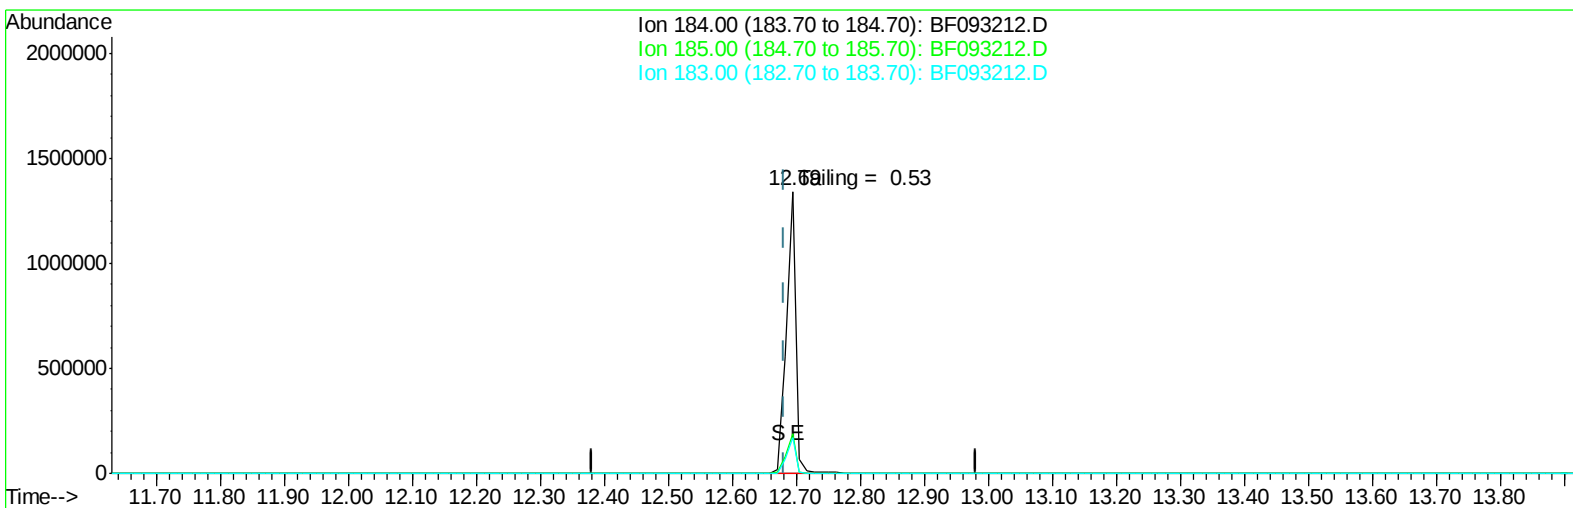

TIC: BF093212.D

(76) Benzidine

12.694min (+0.011) 22858.61ng

response 1395839

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.21
183.00	11.50	12.84
0.00	0.00	0.00