

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022717\
 Data File : BF093235.D
 Acq On : 28 Feb 2017 5:22
 Operator : SJ/MA
 Sample : I1972-05 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2B21-BASE-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.664	135	138	141	rVB	9975	16834	1.37%	0.175%
2	4.967	250	252	263	rVB	60286	78193	6.38%	0.812%
3	5.356	284	286	290	rBV	25417	37070	3.02%	0.385%
4	5.413	290	291	300	rVB2	169420	246385	20.09%	2.558%
5	5.630	308	310	314	rVB2	21721	29945	2.44%	0.311%
6	6.476	381	384	392	rBV	164909	267914	21.84%	2.781%
7	6.590	392	394	397	rVV	294947	274311	22.37%	2.848%
8	6.647	397	399	402	rVB2	17143	25275	2.06%	0.262%
9	6.819	412	414	417	rBV	1132509	955331	77.89%	9.917%
10	6.979	426	428	430	rBV	176435	194776	15.88%	2.022%
11	7.390	462	464	468	rBV	138127	150863	12.30%	1.566%
12	8.110	524	527	529	rBV	1010451	1226455	100.00%	12.732%
13	8.659	572	575	577	rBV4	5542	17181	1.40%	0.178%
14	8.819	588	589	590	rBV	26798	19543	1.59%	0.203%
15	8.910	595	597	601	rBV	12362	24121	1.97%	0.250%
16	9.173	618	620	623	rBV	196637	276269	22.53%	2.868%
17	9.253	625	627	631	rBV4	19811	54928	4.48%	0.570%
18	9.516	648	650	651	rBV2	17077	16232	1.32%	0.169%
19	9.585	652	656	657	rVB3	27687	51470	4.20%	0.534%
20	9.722	665	668	669	rBV	71356	88235	7.19%	0.916%
21	9.859	677	680	682	rBV	1307796	1170965	95.48%	12.156%
22	9.893	682	683	687	rVB4	23870	31248	2.55%	0.324%
23	9.962	687	689	692	rBV3	11990	23437	1.91%	0.243%
24	10.191	706	709	711	rBV3	20485	50304	4.10%	0.522%
25	10.259	713	715	716	rBV2	34516	36226	2.95%	0.376%
26	10.408	726	728	731	rBV2	18407	37099	3.02%	0.385%
27	10.648	747	749	751	rBV	117093	105775	8.62%	1.098%
28	10.762	757	759	763	rVB2	47774	82544	6.73%	0.857%
29	11.345	807	810	811	rBV	1112244	1007900	82.18%	10.463%
30	11.368	811	812	814	rVV	174530	131752	10.74%	1.368%
31	11.414	814	816	818	rVV	41130	50676	4.13%	0.526%
32	11.951	861	863	865	rBV2	49265	78977	6.44%	0.820%
33	12.431	903	905	906	rVB2	68762	61911	5.05%	0.643%
34	12.557	914	916	918	rVB	170630	139578	11.38%	1.449%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022717\
Data File : BF093235.D
Acq On : 28 Feb 2017 5:22
Operator : SJ/MA
Sample : I1972-05 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2B21-BASE-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.785	934	936	940 rBV	310766	390435	31.83%	4.053%
36	12.922	946	948	952 rVB	174154	227637	18.56%	2.363%
37	13.985	1039	1041	1045 rBV	887792	1083004	88.30%	11.243%
38	15.425	1164	1167	1174 rVB	533718	872179	71.11%	9.054%


Sum of corrected areas: 9632978

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022717\
Data File : BF093235.D
Acq On : 28 Feb 2017 5:22
Operator : SJ/MA
Sample : I1972-05 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2B21-BASE-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

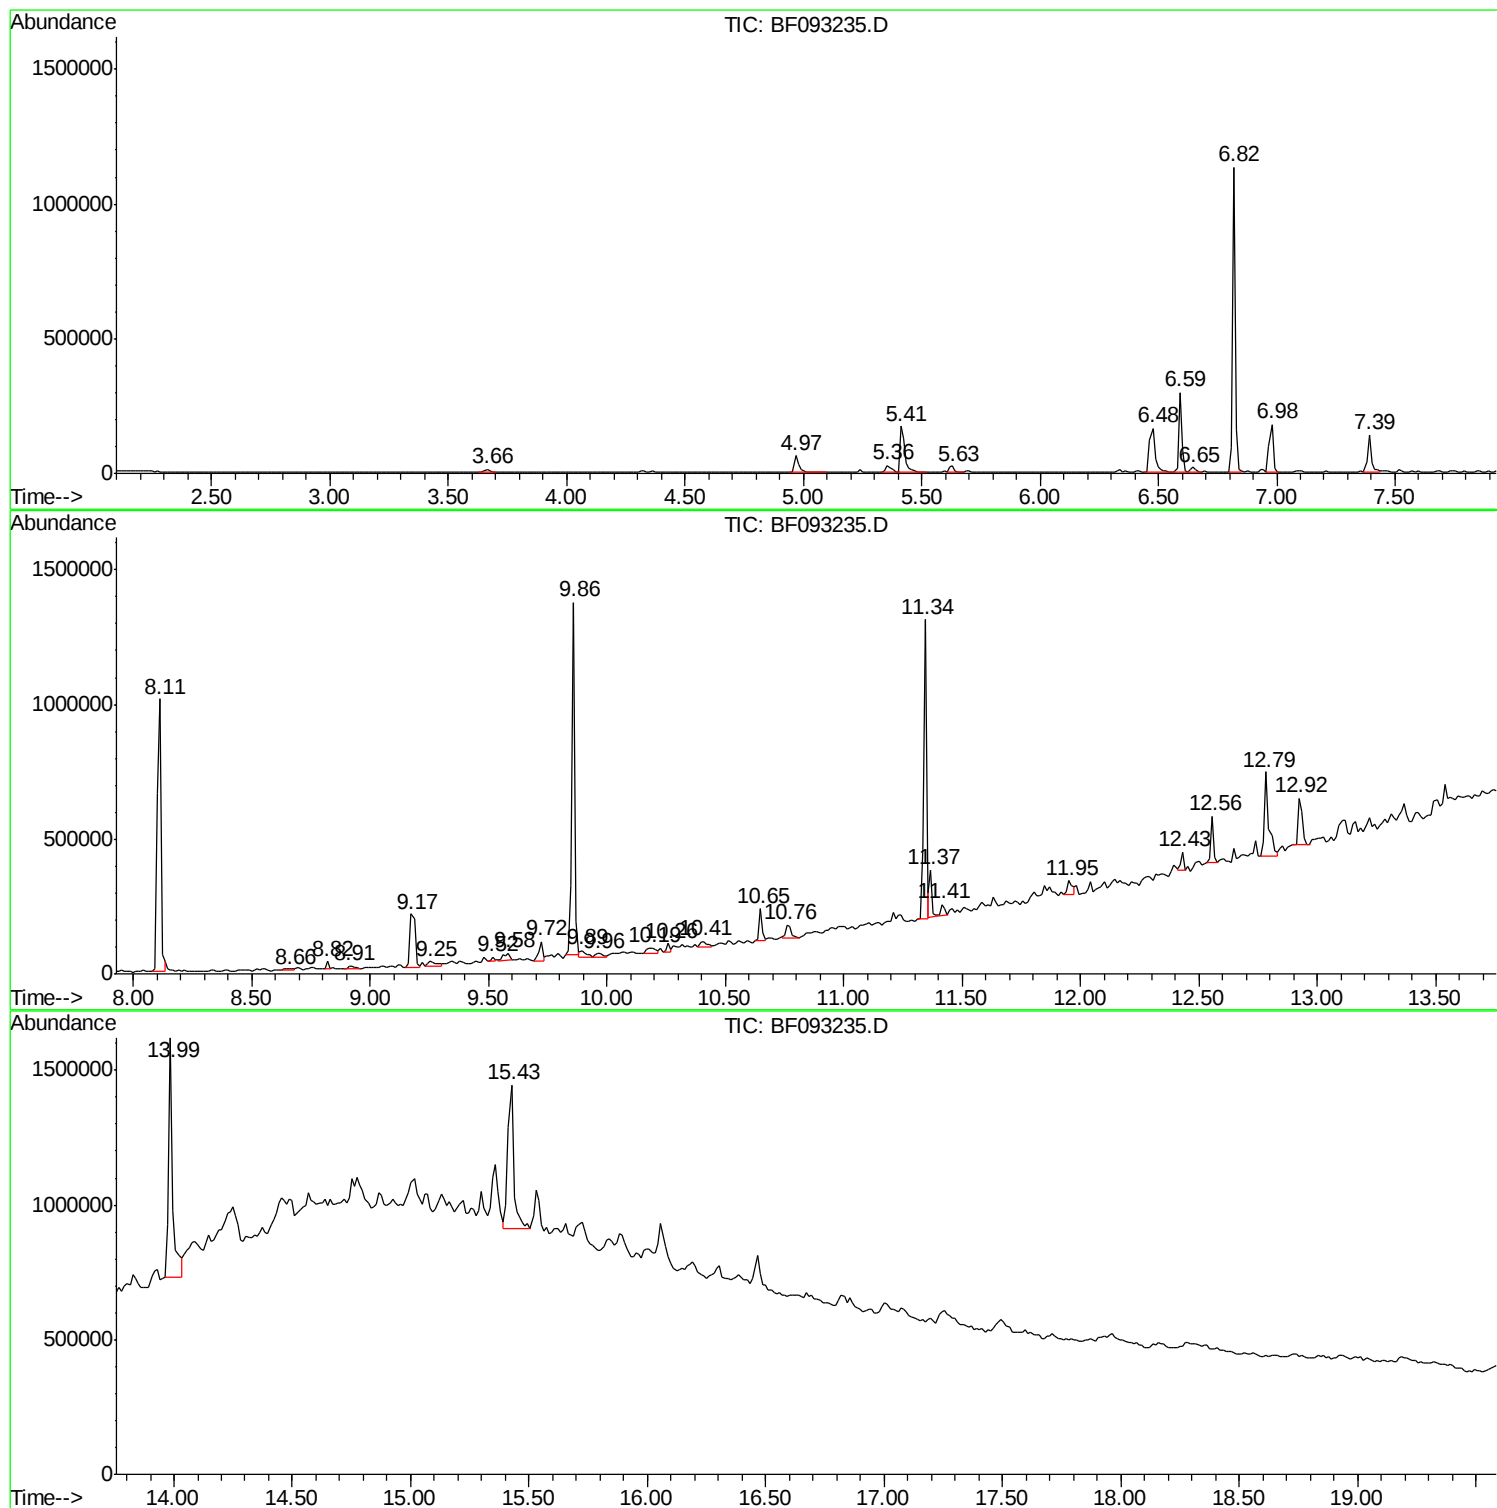

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022717\
Data File : BF093235.D
Acq On : 28 Feb 2017 5:22
Operator : SJ/MA
Sample : I1972-05 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2B21-BASE-2










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.59	5.74 ng	274311	1,4-Dichlorobenzene-d4	6.82

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	12
4			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

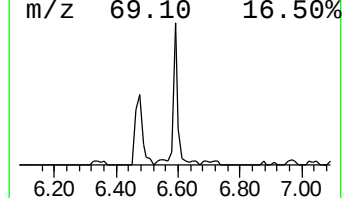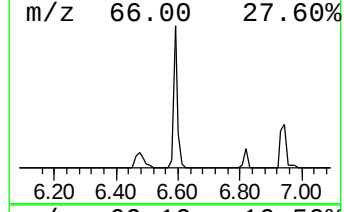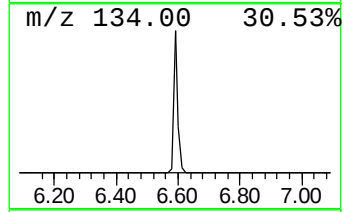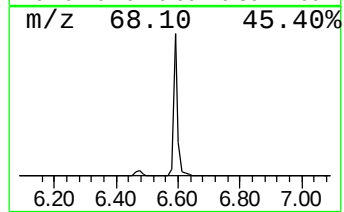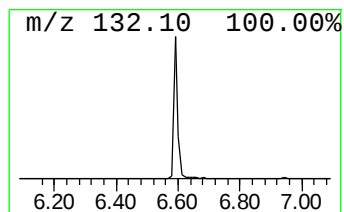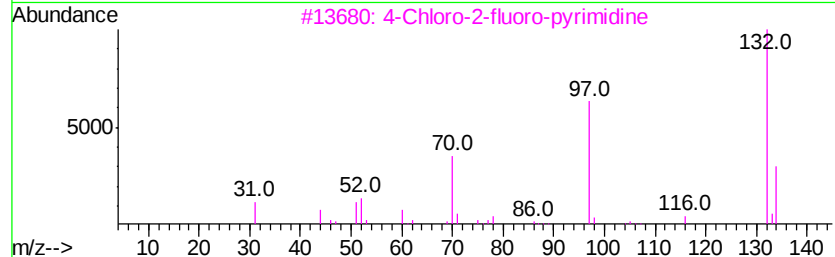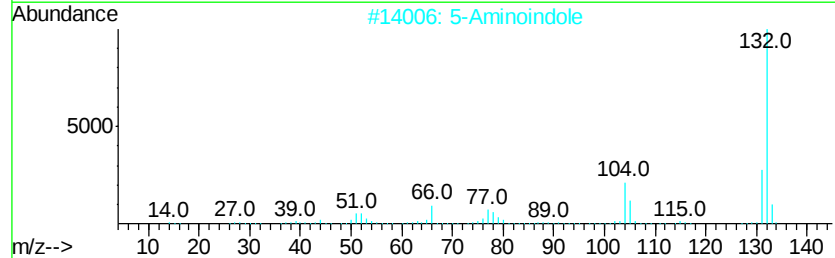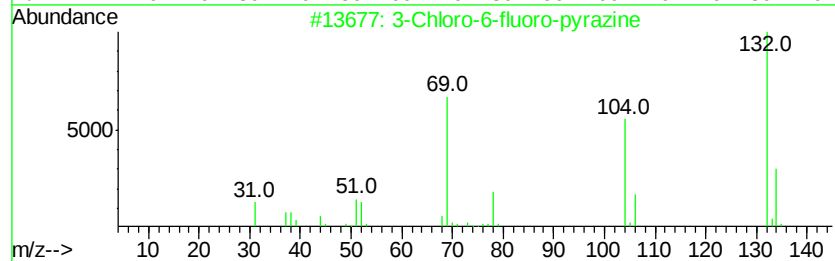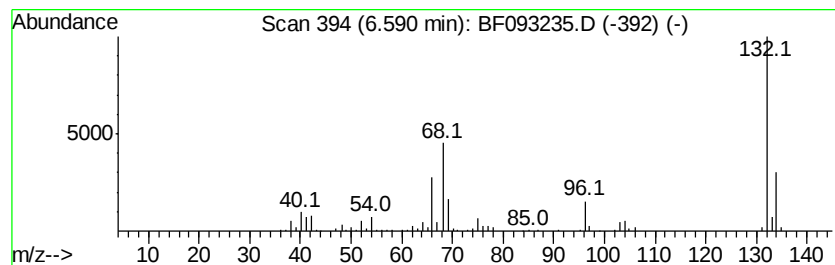

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022717\
Data File : BF093235.D
Acq On : 28 Feb 2017 5:22
Operator : SJ/MA
Sample : I1972-05 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2B21-BASE-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.59	6.59	5.7	ng	274311	1	6.82	955331	20.0