

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022718\
 Data File : BF103288.D
 Acq On : 28 Feb 2018 3:21
 Operator : SJ/JU
 Sample : J1683-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Feb 28 03:58:48 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 17:05:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	142475	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	534393	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	222973	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	318332	20.00	ng	0.00
75) Chrysene-d12	14.05	240	243111	20.00	ng	0.00
86) Perylene-d12	15.56	264	186837	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	432884	45.95	ng	0.00
7) Phenol-d6	6.50	99	354478	30.75	ng	0.00
23) Nitrobenzene-d5	7.45	82	571907	61.12	ng	0.00
41) 2,4,6-Tribromophenol	10.71	330	164718	87.28	ng	0.00
44) 2-Fluorobiphenyl	9.23	172	966449	71.96	ng	0.00
78) Terphenyl-d14	12.99	244	681583	67.39	ng	0.00
Target Compounds						
10) Phenol	6.52	94	53547	4.00	ng	Qvalue 92
18) Hexachloroethane	7.40	117	158834	38.91	ng	# 1
22) Acetophenone	7.26	105	304935	24.45	ng	# 58
24) Nitrobenzene	7.45	77	33786	3.28	ng	# 8
25) Isophorone	7.45	82	571875	31.03	ng	# 64
31) Naphthalene	8.18	128	421825	16.12	ng	97
32) Benzoic acid	7.95	122	5030	7.70	ng	# 1
35) Caprolactam	8.61	113	5442	2.18	ng	# 1
47) 2-Nitroaniline	9.47	65	48211	8.81	ng	# 22
49) Dimethylphthalate	9.63	163	51990	2.91	ng	# 57
53) 2,4-Dinitrophenol	10.12	184	106	9.69	ng	# 1
64) 4,6-Dinitro-2-methylphenol	10.71	198	590	5.22	ng	# 1
66) 4-Bromophenyl-phenylether	10.71	248	11543	3.48	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022718\
Data File : BF103288.D
Acq On : 28 Feb 2018 3:21
Operator : SJ/JU
Sample : J1683-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Feb 28 03:58:48 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 17:05:20 2018
Response via : Initial Calibration

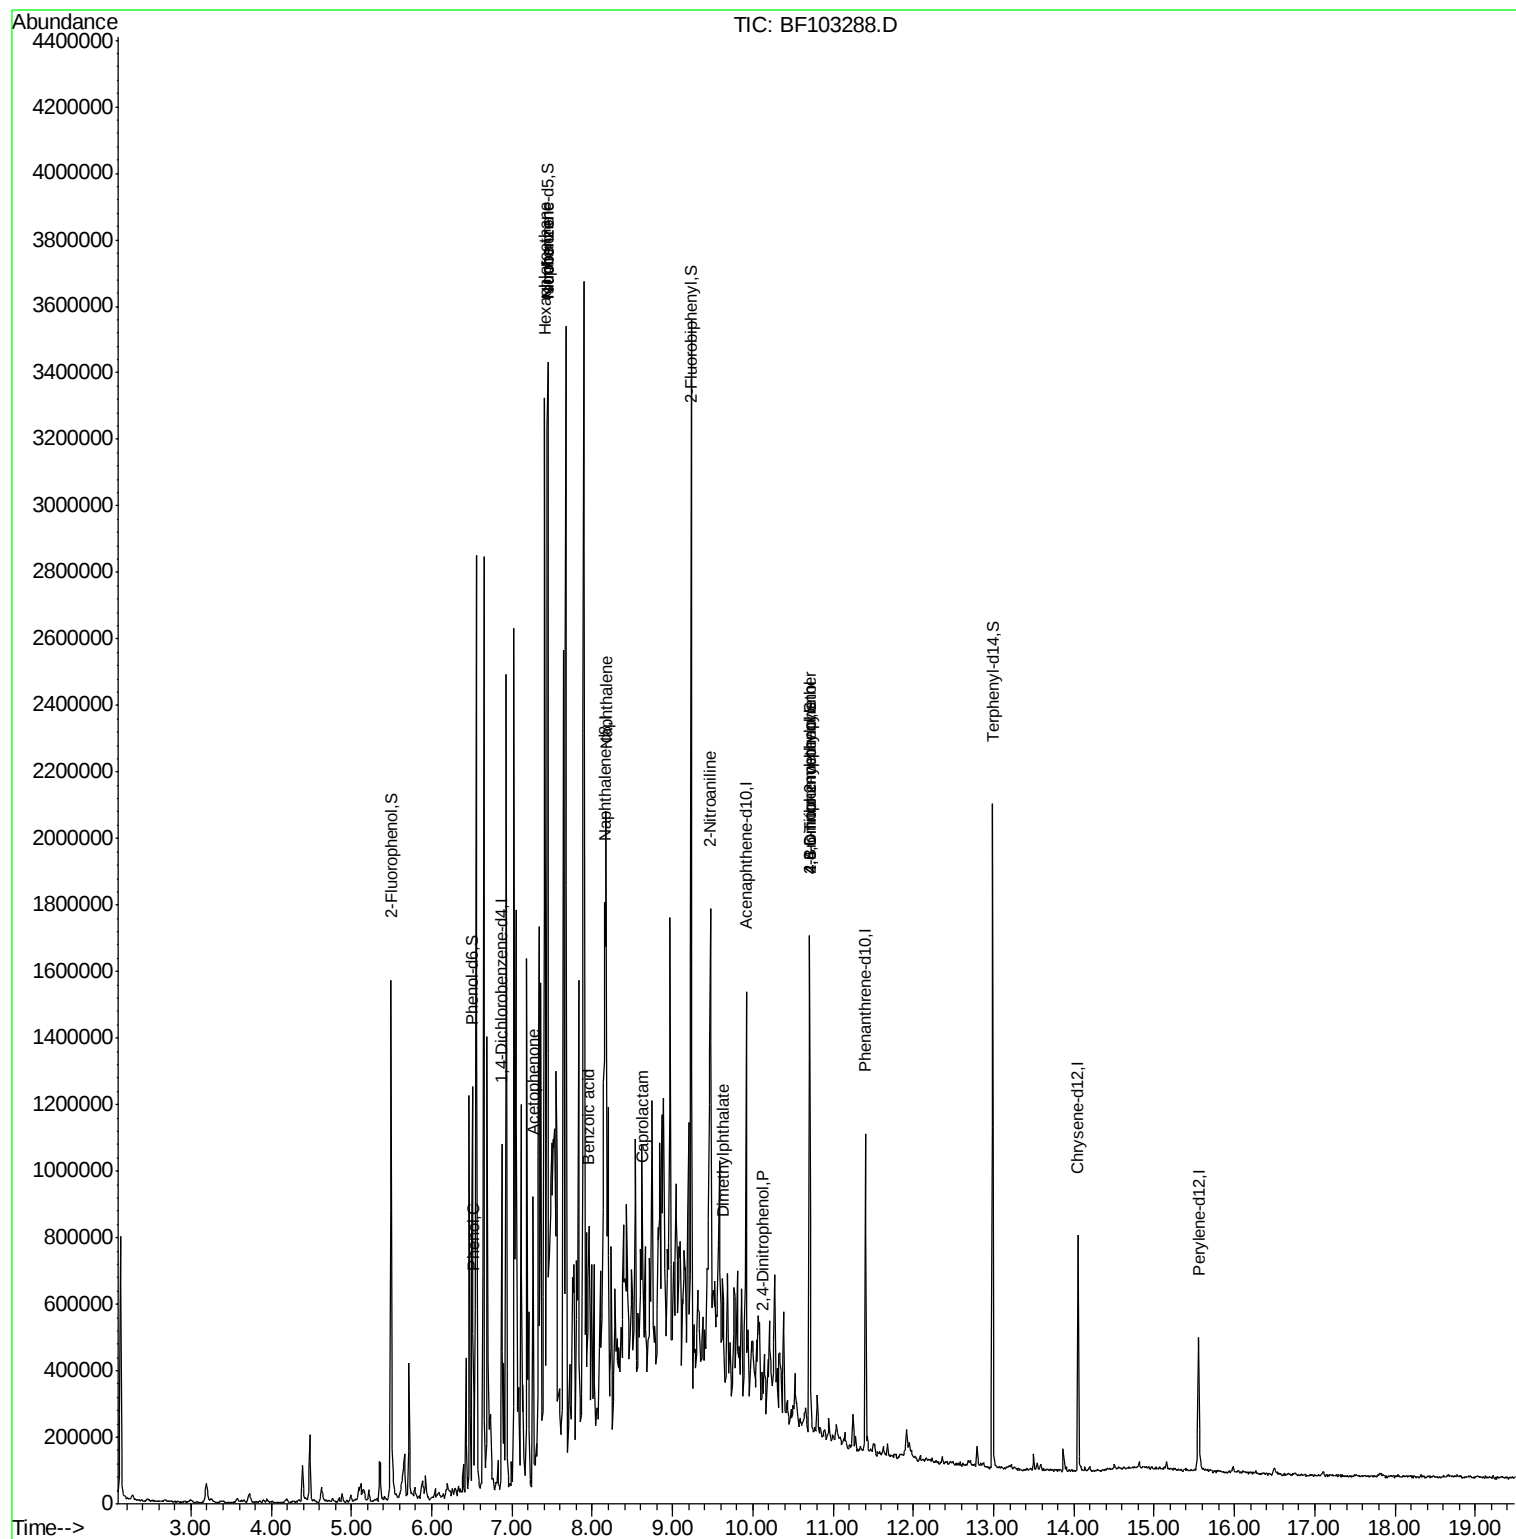




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.87 min Scan# 814
Delta R.T. -0.00 min
Lab File: BF103288.D
Acq: 28 Feb 2018 3:21

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.6	124.6	186.8
115	62.4	50.1	75.1




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

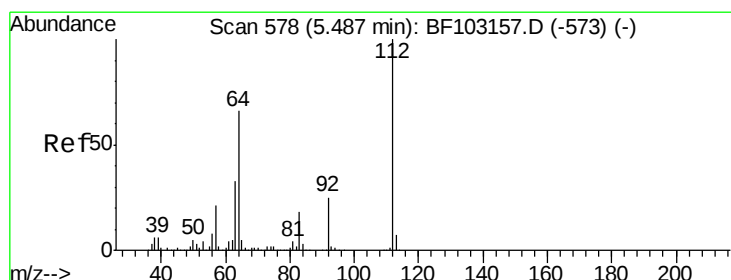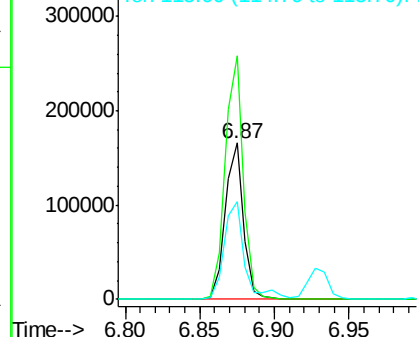



#5


2-Fluorophenol
Concen: 45.95 ng
RT: 5.49 min Scan# 579
Delta R.T. -0.00 min
Lab File: BF103288.D
Acq: 28 Feb 2018 3:21

Tgt Ion	Ratio	Lower	Upper
112	100		
64	68.0	47.9	71.9
63	35.4	23.7	35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

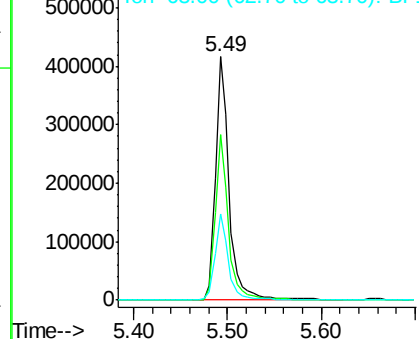

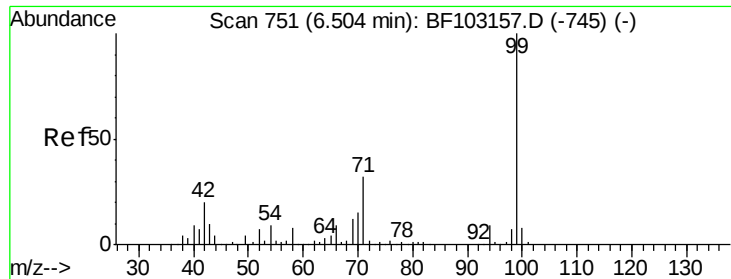

#7

Phenol-d6

Concen: 30.75 ng

RT: 6.50 min Scan# 751

Delta R.T. -0.01 min

Lab File: BF103288.D

Acq: 28 Feb 2018 3:21

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 354478

Ion Ratio Lower Upper




99 100

42 23.4 14.5 21.7#

71 53.4 25.4 38.0#

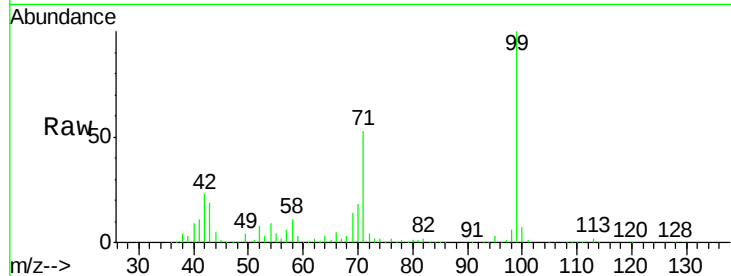

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

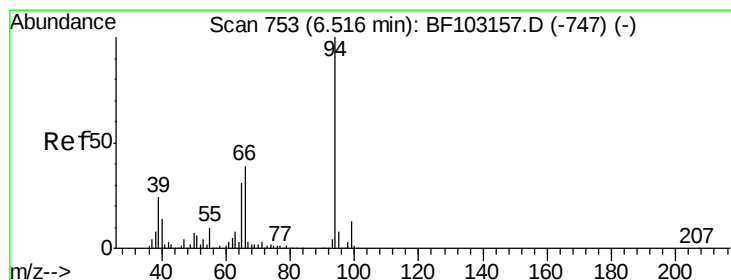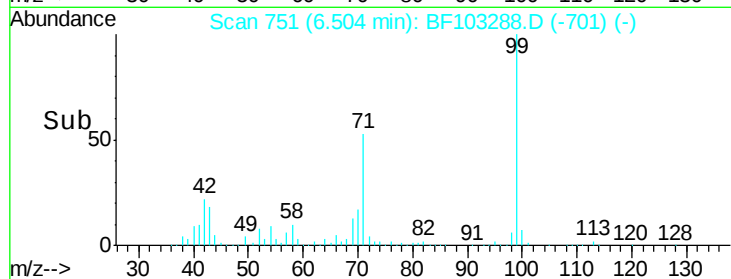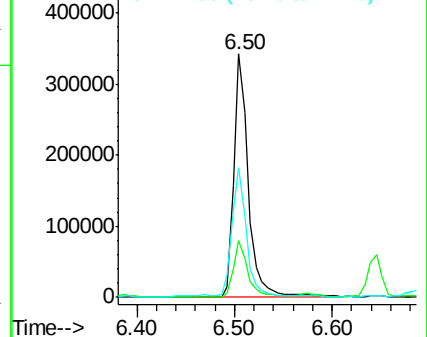

#10

Phenol

Concen: 4.00 ng

RT: 6.52 min Scan# 754

Delta R.T. -0.00 min

Lab File: BF103288.D

Acq: 28 Feb 2018 3:21


Tgt Ion: 94 Resp: 53547

Ion Ratio Lower Upper



94 100


65 29.0 7.9 47.9

66 43.2 16.2 56.2



Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1




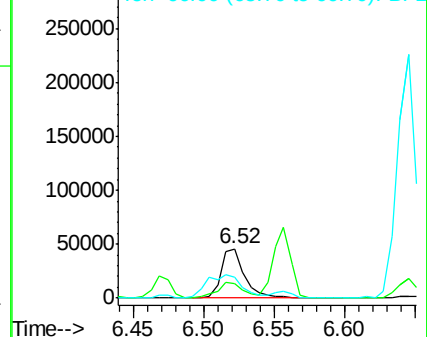




#18
Hexachloroethane
Concen: 38.91 ng
RT: 7.40 min Scan# 904
Delta R.T. 0.02 min
Lab File: BF103288.D
Acq: 28 Feb 2018 3:21




Instrument :
BNA_F
ClientSampleId :


Tot Ion:117 Resp: 158834
Ion Ratio Lower Upper
117 100
119 683.0 75.8 113.8#
201 0.0 75.7 113.5#

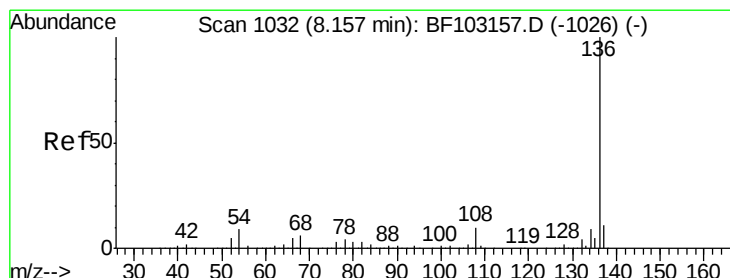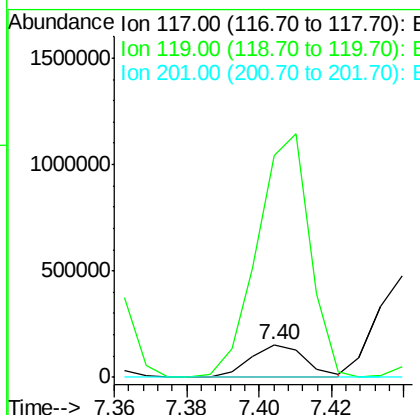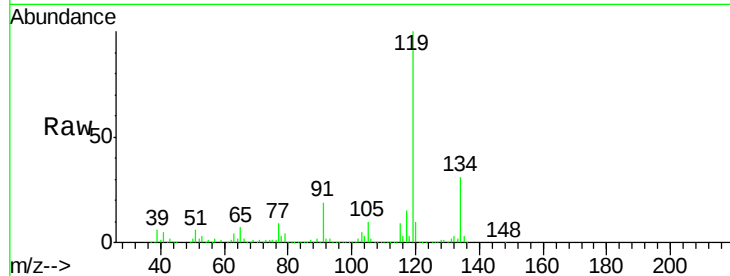

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.16 min Scan# 1032
Delta R.T. -0.00 min
Lab File: BF103288.D
Acq: 28 Feb 2018 3:21

Tgt Ion:136 Resp: 534393
Ion Ratio Lower Upper
136 100
137 10.8 8.9 13.3
54 10.0 6.6 9.8#
68 7.0 5.0 7.4

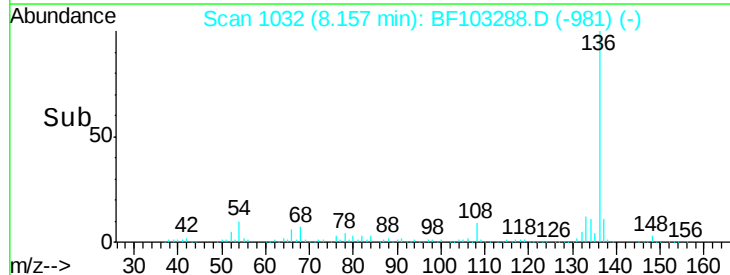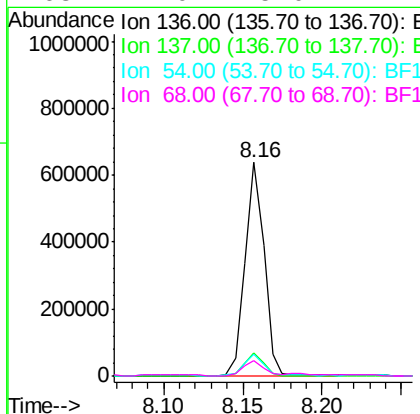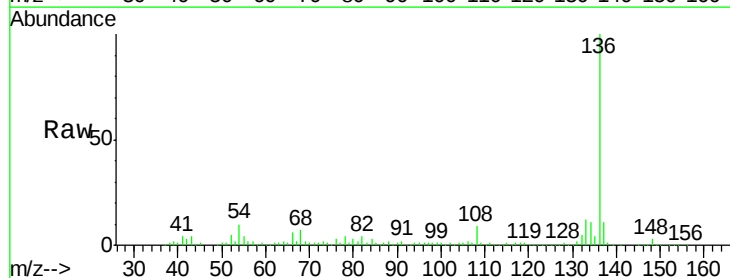



#22

Acetophenone

Concen: 24.45 ng

RT: 7.26 min Scan# 880

Delta R.T. -0.02 min

Lab File: BF103288.D

Acq: 28 Feb 2018 3:21

Instrument :

BNA_F

ClientSampled :

Tot Ion: 105 Resp: 304935


Ion Ratio Lower Upper

105 100

71 0.7 4.4 6.6#

51 3.9 22.3 33.5#

120 0.2 16.9 25.3#



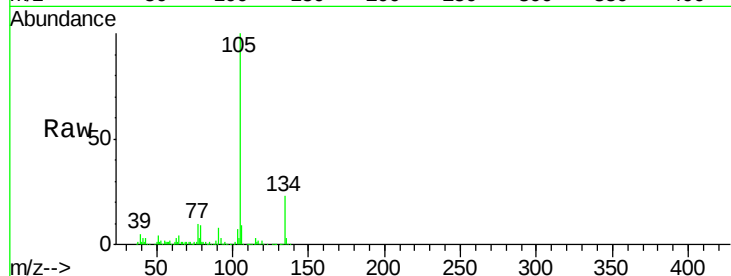


Abundance Ion 105.00 (104.70 to 105.70): E

Ion 71.00 (70.70 to 71.70): BF1

Ion 51.00 (50.70 to 51.70): BF1

Ion 120.00 (119.70 to 120.70): E

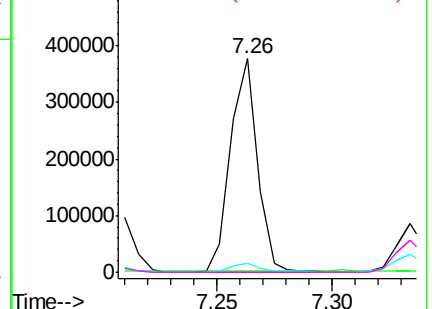

#23

Nitrobenzene-d5

Concen: 61.12 ng

RT: 7.45 min Scan# 911

Delta R.T. -0.00 min

Lab File: BF103288.D

Acq: 28 Feb 2018 3:21


Tgt Ion: 82 Resp: 571907

Ion Ratio Lower Upper

82 100

128 49.3 36.1 54.1



54 57.9 41.4 62.2




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

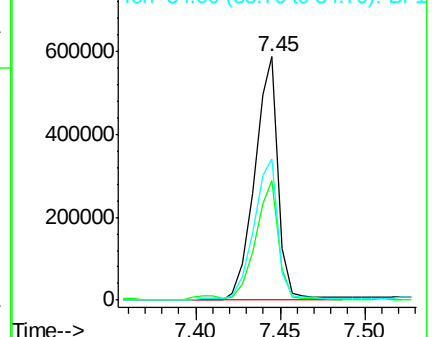



#24

Nitrobenzene

Concen: 3.28 ng

RT: 7.45 min Scan# 911


Delta R.T. -0.02 min

Lab File: BF103288.D




Acq: 28 Feb 2018 3:21

Instrument :
BNA_F
ClientSampleId :

Tot Ion	77	123	65	Resp	33786	Lower	Upper
Ion Ratio	100	1.3	84.4				
		37.9	11.0				
		56.9#	16.4#				

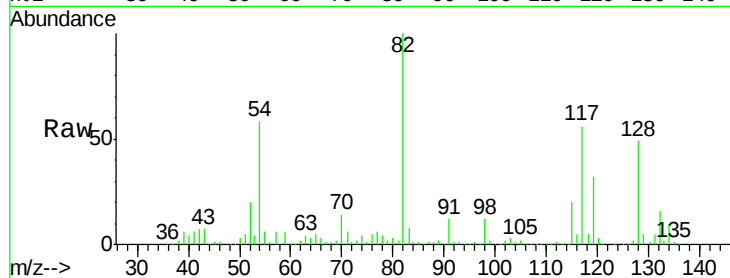

Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 123.00 (122.70 to 123.70): BF1
Ion 65.00 (64.70 to 65.70): BF1

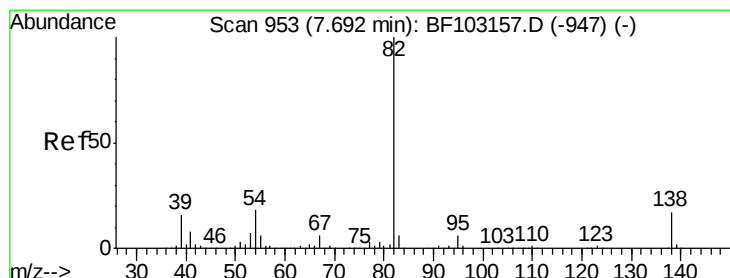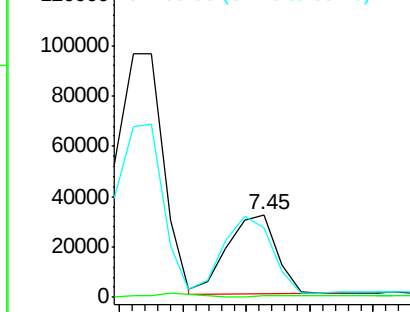

#25

Isophorone

Concen: 31.03 ng


RT: 7.45 min Scan# 911

Delta R.T. -0.25 min



Lab File: BF103288.D


Acq: 28 Feb 2018 3:21

Tgt Ion	82	95	138	Resp	571875	Lower	Upper
Ion Ratio	100	0.2	0.0				
		5.2	14.9				
		7.8#	22.3#				

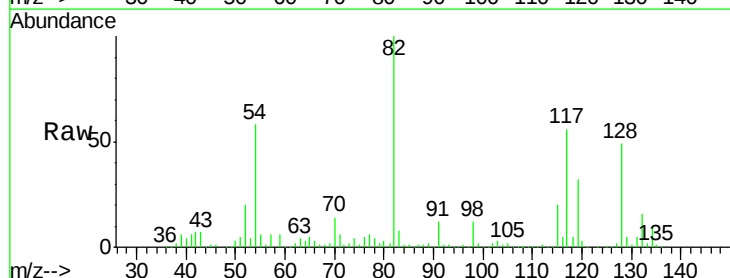

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1



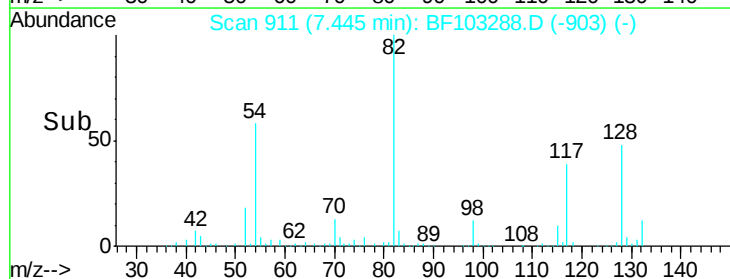
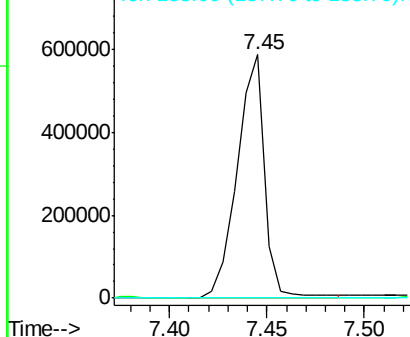




#31
Naphthalene
Concen: 16.12 ng
RT: 8.18 min Scan# 1036
Delta R.T. -0.00 min
Lab File: BF103288.D
Acq: 28 Feb 2018 3:21




Instrument :
BNA_F
ClientSampleId :


Tot Ion:128 Resp: 421825
Ion Ratio Lower Upper
128 100
129 12.9 8.8 13.2
127 14.2 10.9 16.3

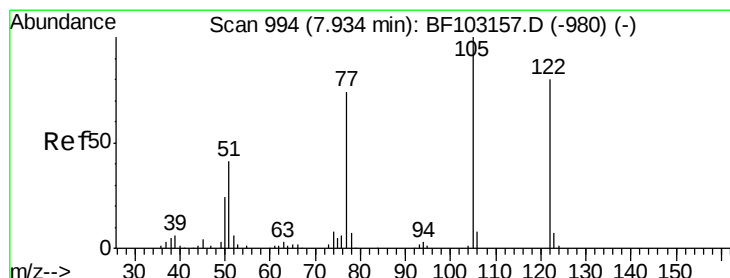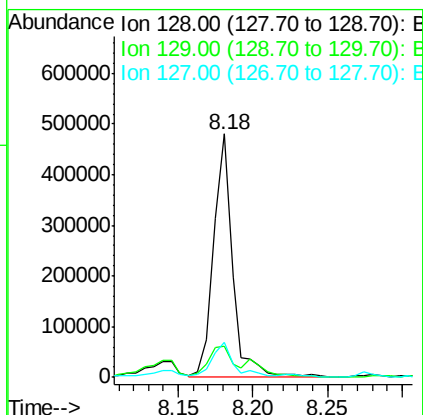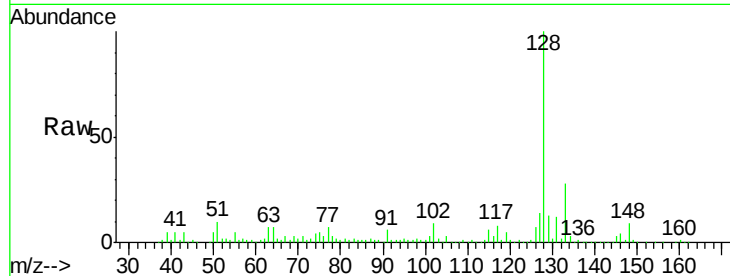

#32
Benzoic acid
Concen: 7.70 ng
RT: 7.95 min Scan# 997
Delta R.T. 0.01 min
Lab File: BF103288.D
Acq: 28 Feb 2018 3:21

Tgt Ion:122 Resp: 5030
Ion Ratio Lower Upper
122 100
105 154.5 101.1 141.1#
77 443.4 70.7 110.7#



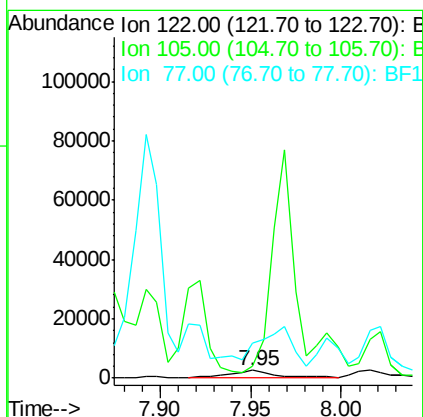
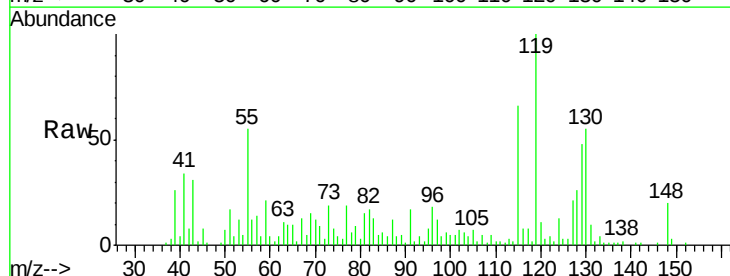




#35
 Caprolactam
 Concen: 2.18 ng
 RT: 8.61 min Scan# 1109
 Delta R.T. -0.01 min
 Lab File: BF103288.D
 Acq: 28 Feb 2018 3:21




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:113 Resp: 5442
 Ion Ratio Lower Upper
 113 100
 55 685.5 163.3 203.3#
 56 220.9 115.7 155.7#

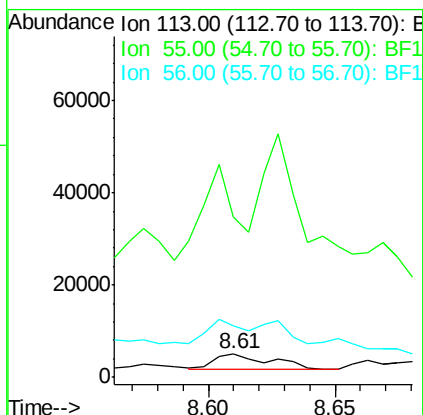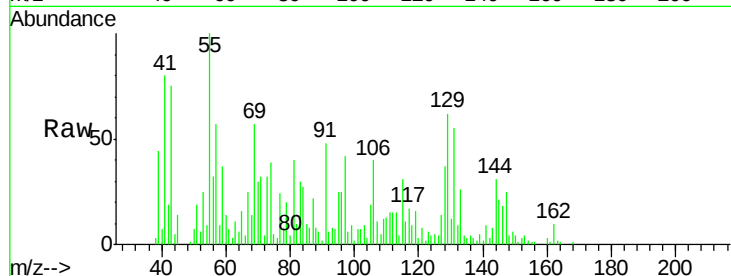

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.00 min
 Lab File: BF103288.D
 Acq: 28 Feb 2018 3:21

Tgt Ion:164 Resp: 222973
 Ion Ratio Lower Upper
 164 100
 162 105.1 86.1 129.1
 160 49.8 38.3 57.5

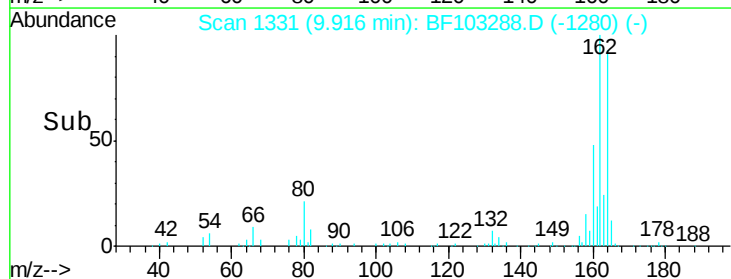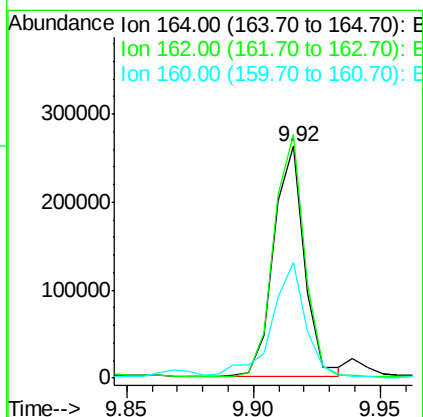




#41
 2,4,6-Tribromophenol
 Concen: 87.28 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.00 min
 Lab File: BF103288.D
 Acq: 28 Feb 2018 3:21

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	103.0	77.0	115.6
141	40.4	29.9	44.9



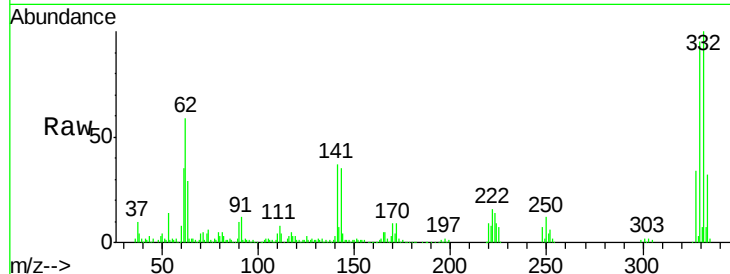


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

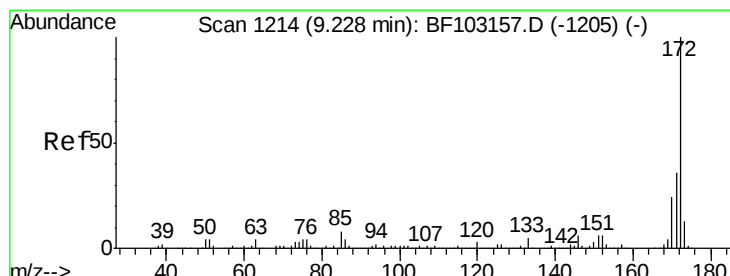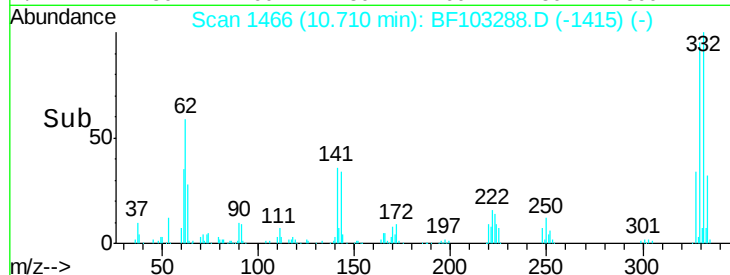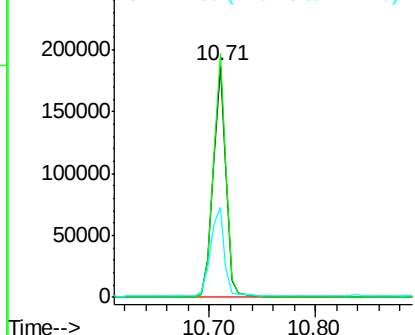

#44
 2-Fluorobiphenyl
 Concen: 71.96 ng
 RT: 9.23 min Scan# 1215
 Delta R.T. -0.00 min
 Lab File: BF103288.D
 Acq: 28 Feb 2018 3:21




Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.7	44.5
170	24.3	19.6	29.4


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

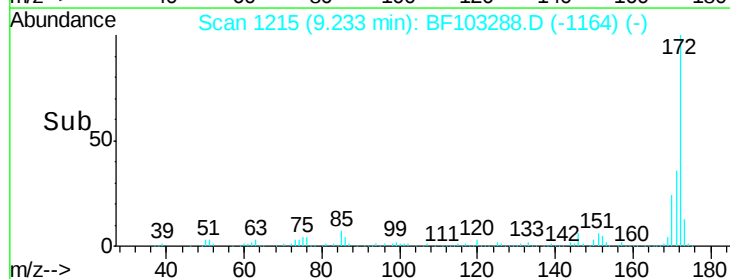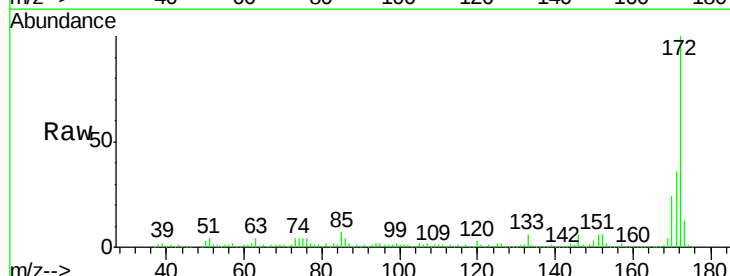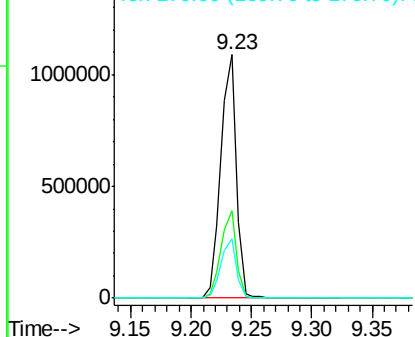

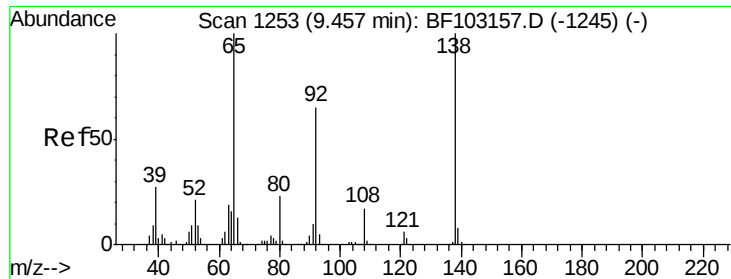

#47

2-Nitroaniline

Concen: 8.81 ng

RT: 9.47 min Scan# 1256

Delta R.T. 0.01 min

Lab File: BF103288.D

Acq: 28 Feb 2018 3:21

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 65 Resp: 48211

Ion Ratio Lower Upper

65 100

92 37.6 55.8 83.6#




138 3.8 91.2 136.8#

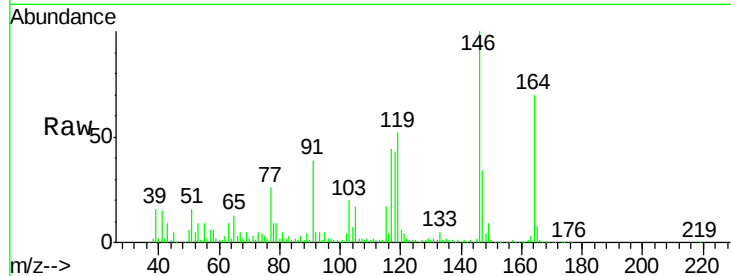

Abundance Ion 65.00 (64.70 to 65.70): BF1

Ion 92.00 (91.70 to 92.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

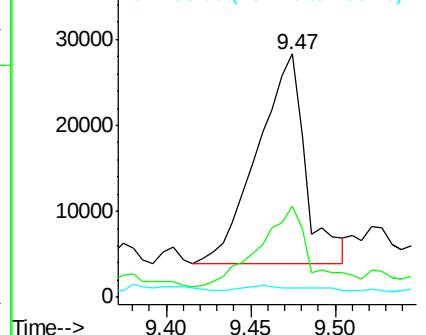

#49

Dimethylphthalate

Concen: 2.91 ng

RT: 9.63 min Scan# 1282

Delta R.T. -0.01 min

Lab File: BF103288.D

Acq: 28 Feb 2018 3:21


Tgt Ion: 163 Resp: 51990

Ion Ratio Lower Upper

163 100

194 3.1 2.7 4.1



164 31.4 8.2 12.2#




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E




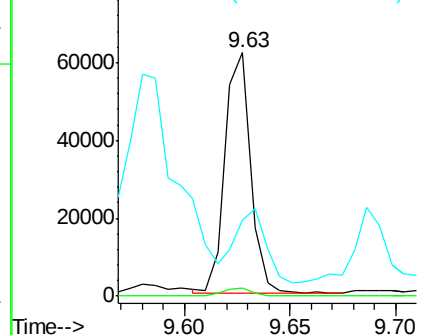




#53
 2,4-Dinitrophenol
 Concen: 9.69 ng
 RT: 10.12 min Scan# 1366
 Delta R.T. 0.14 min
 Lab File: BF103288.D
 Acq: 28 Feb 2018 3:21




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:184 Resp: 106
 Ion Ratio Lower Upper
 184 100
 63 955.1 54.2 81.2#
 154 202.7 184.0 276.0

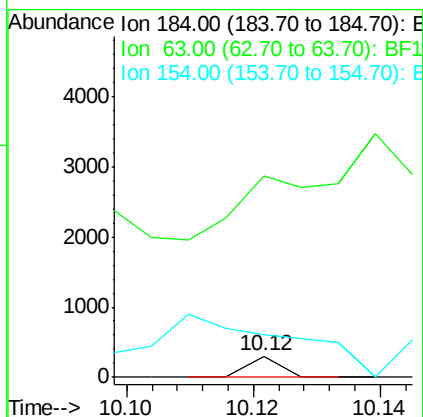

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.40 min Scan# 1584
 Delta R.T. -0.00 min
 Lab File: BF103288.D
 Acq: 28 Feb 2018 3:21

Tgt Ion:188 Resp: 318332
 Ion Ratio Lower Upper
 188 100
 94 12.6 8.5 12.7
 80 13.4 9.2 13.8

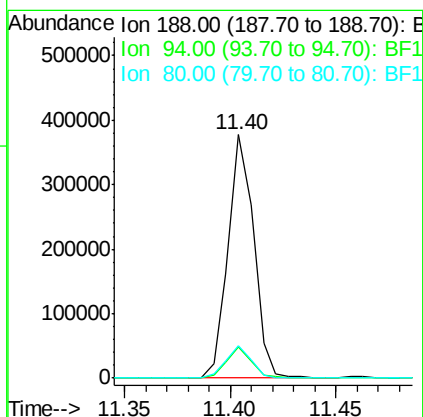







#64
 4,6-Dinitro-2-methylphenol
 Concen: 5.22 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. 0.18 min
 Lab File: BF103288.D
 Acq: 28 Feb 2018 3:21

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:198 Resp: 590
 Ion Ratio Lower Upper
 198 100
 51 426.4 37.7 77.7#
 105 439.7 36.3 76.3#

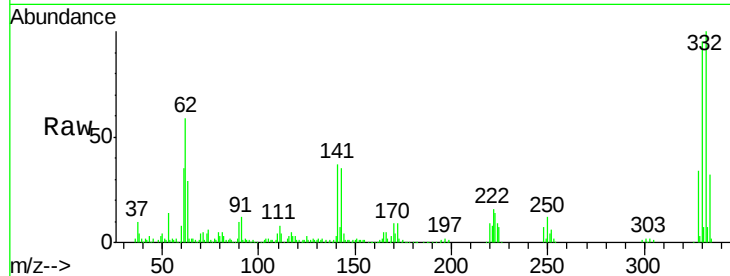


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E

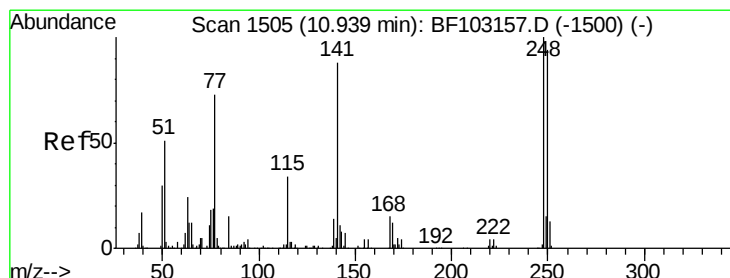
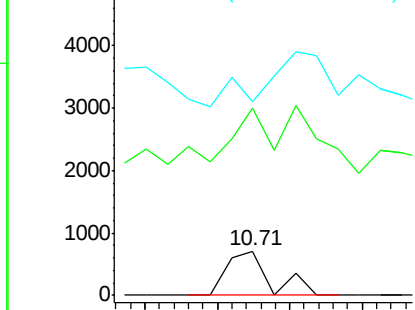



#66
 4-Bromophenyl-phenylether
 Concen: 3.48 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.24 min
 Lab File: BF103288.D
 Acq: 28 Feb 2018 3:21

Tgt Ion:248 Resp: 11543
 Ion Ratio Lower Upper
 248 100
 250 182.9 76.9 115.3#
 141 551.8 74.4 111.6#

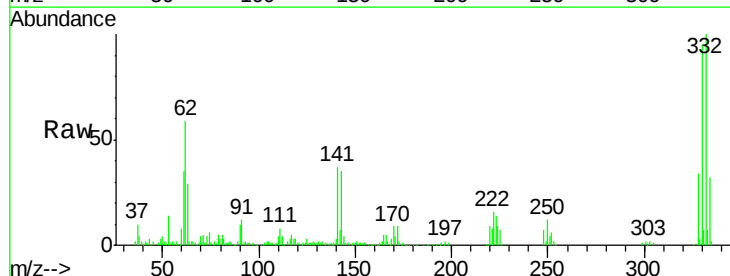

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

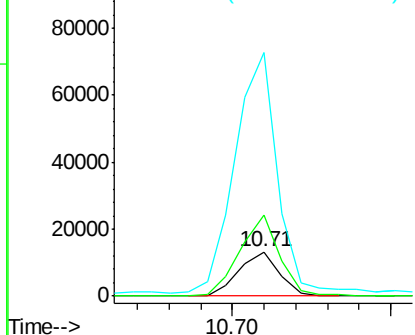



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.05 min Scan# 2034

Delta R.T. -0.01 min

Lab File: BF103288.D

Acq: 28 Feb 2018 3:21

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 243111

Ion Ratio Lower Upper

240 100

120 16.3 9.5 14.3#




236 25.4 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

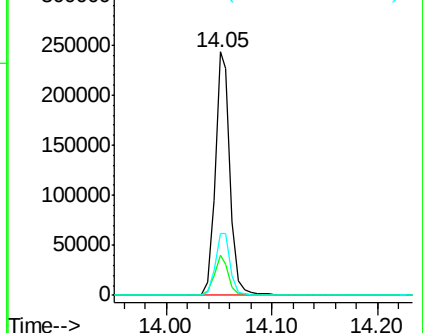

#78

Terphenyl-d14

Concen: 67.39 ng

RT: 12.99 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BF103288.D

Acq: 28 Feb 2018 3:21


Tgt Ion:244 Resp: 681583

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0



122 15.1 11.0 16.4






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

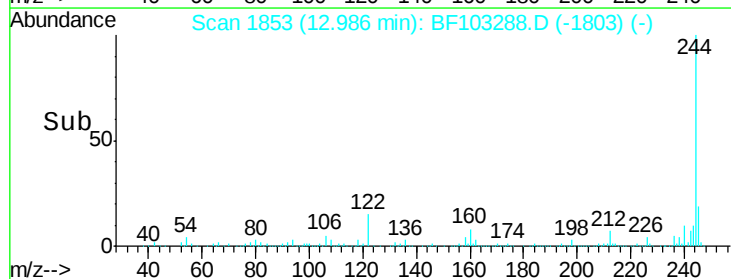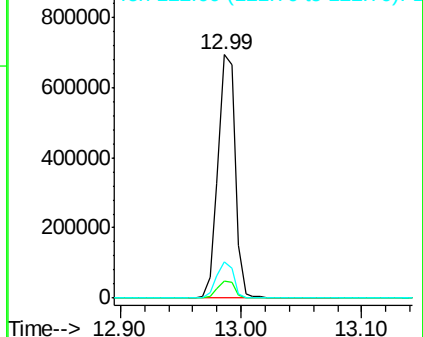

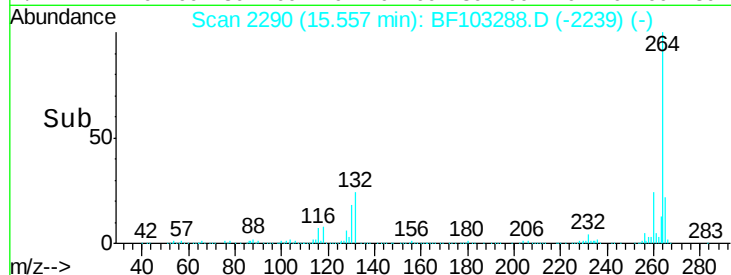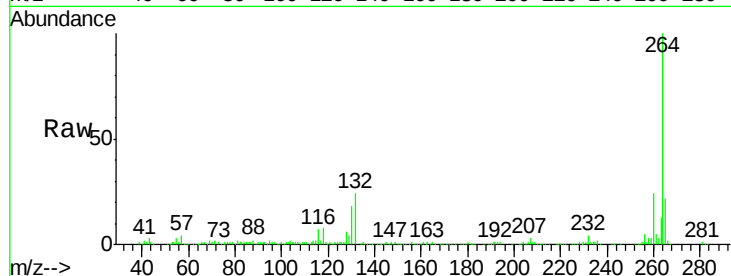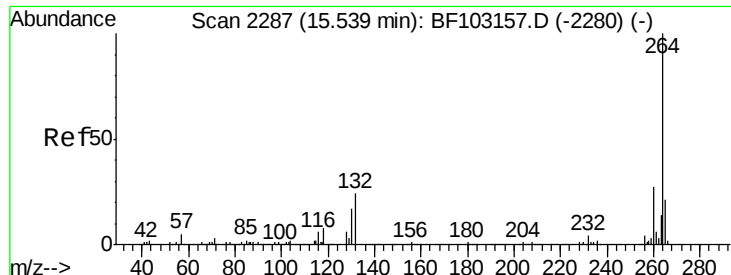

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.56 min Scan# 2290
 Delta R.T. -0.00 min
 Lab File: BF103288.D
 Acq: 28 Feb 2018 3:21

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:	264	Resp:	186837
Ion Ratio	Lower	Upper	
264	100		
260	24.1	19.2	28.8
265	21.7	17.5	26.3

