
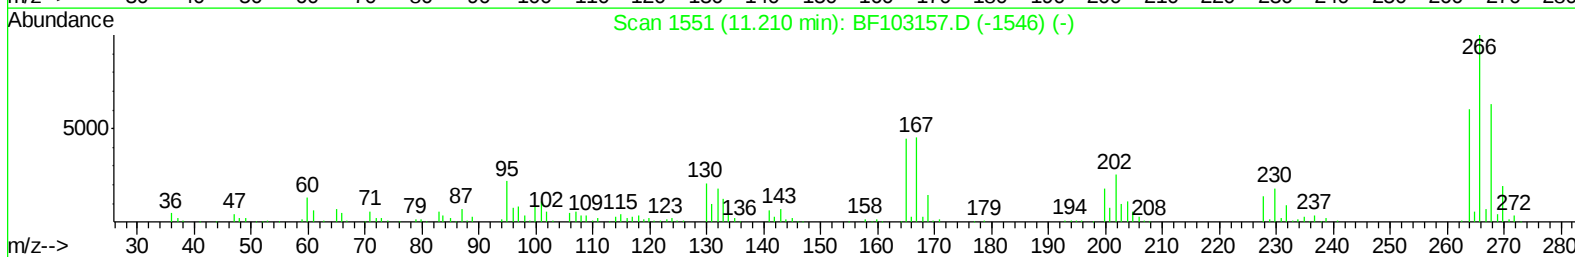
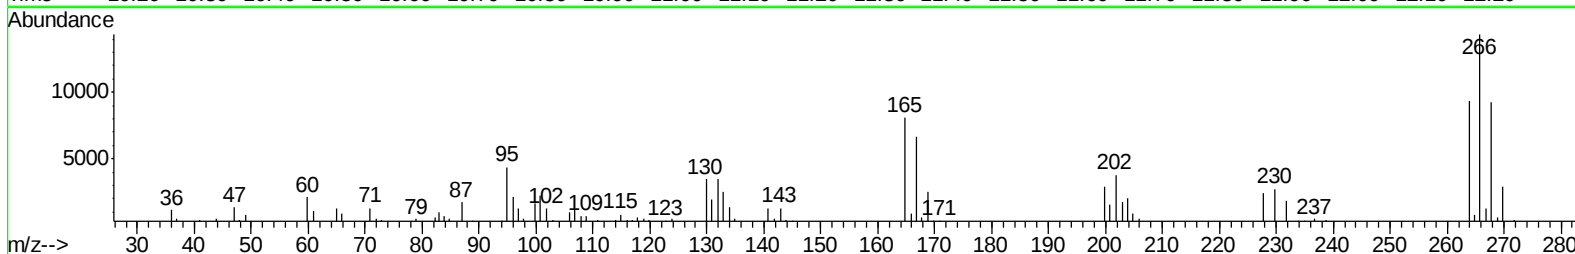


Data Path : Z:\HPCHEM1\BNA F\DATA\BF022718\
Data File : BF103282.D
Acq On : 28 Feb 2018 00:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 05:37:28 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 17:05:20 2018
Response via : Initial Calibration

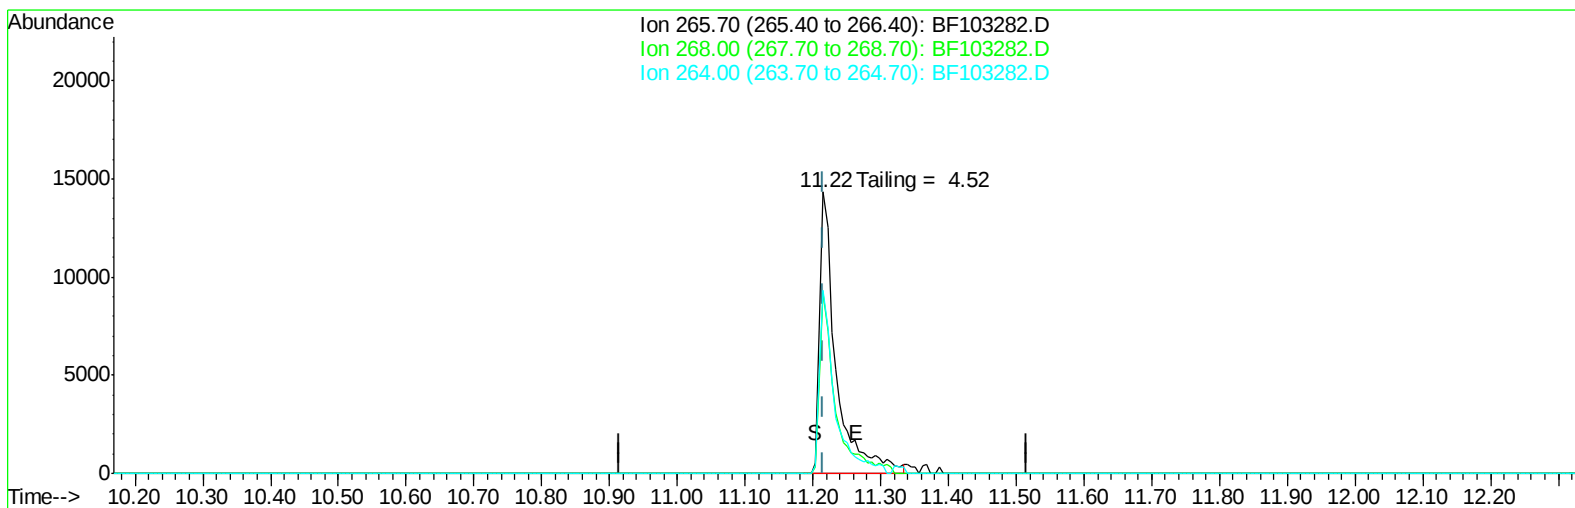

TIC: BF103282.D

(69) Pentachlorophenol (C)




11.216min (-0.000) 33990.95ng

response 23600

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.29
264.00	61.90	64.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022718\
 Data File : BF103282.D
 Acq On : 28 Feb 2018 00:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 05:37:28 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 17:05:20 2018
 Response via : Initial Calibration

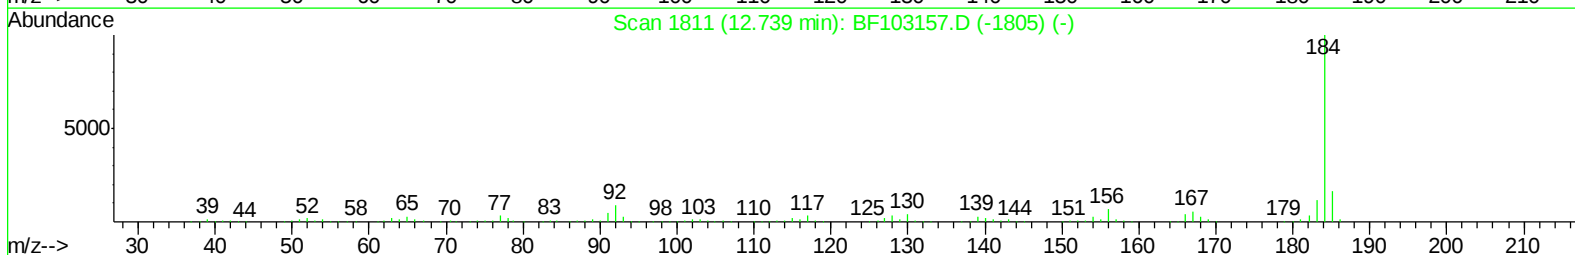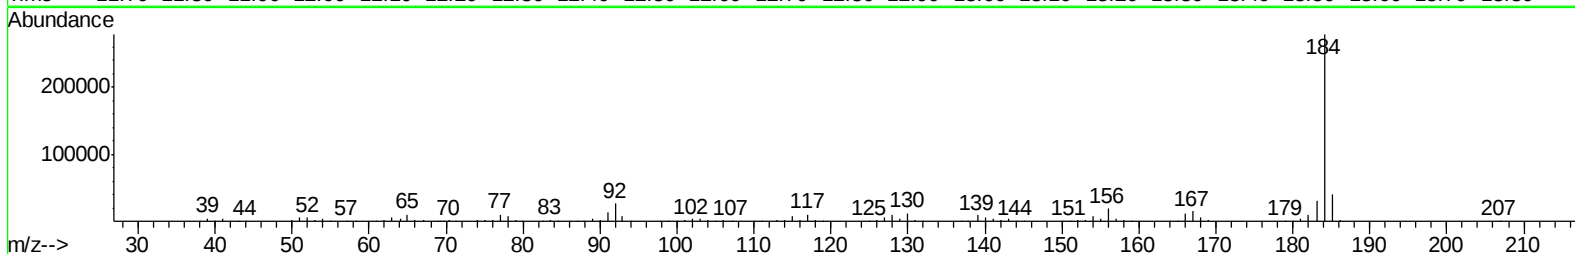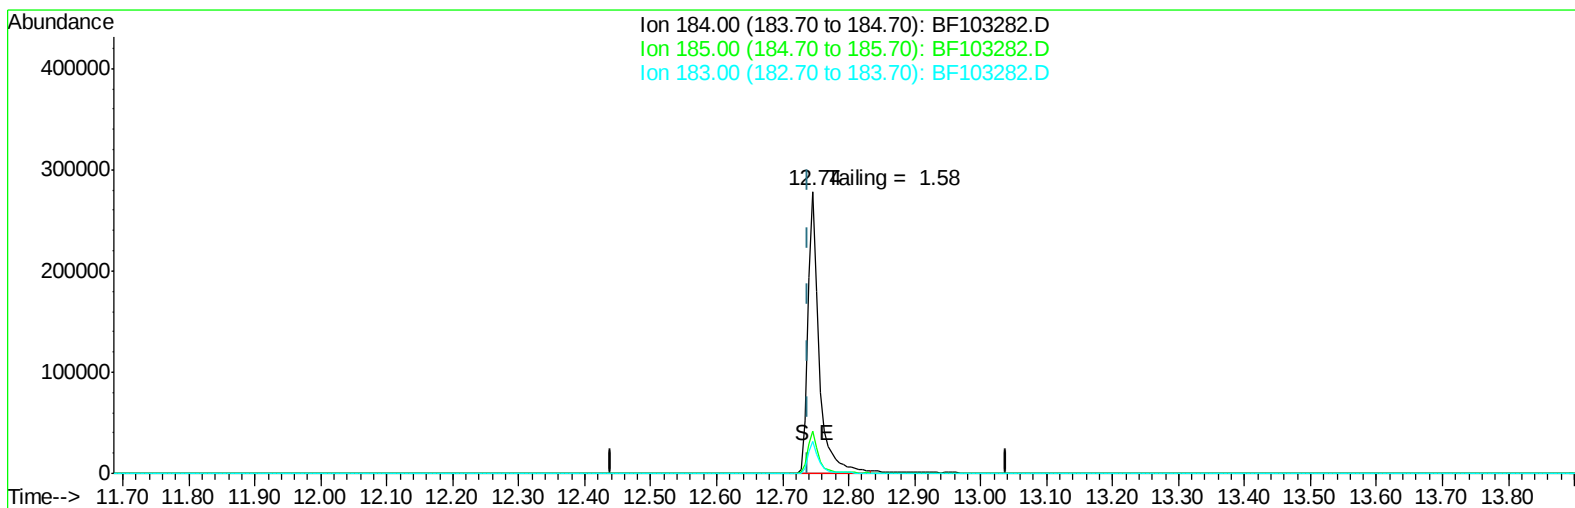

TIC: BF103282.D

(76) Benzidine

12.745min (+0.006) 0.00ng

response 338783

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.81
183.00	11.60	11.21
0.00	0.00	0.00