


Data Path : Z:\HPCHEM1\BNA_F\Data\BF022718\
 Data File : BF103282.D
 Acq On : 28 Feb 2018 00:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 27 17:05:20 2018

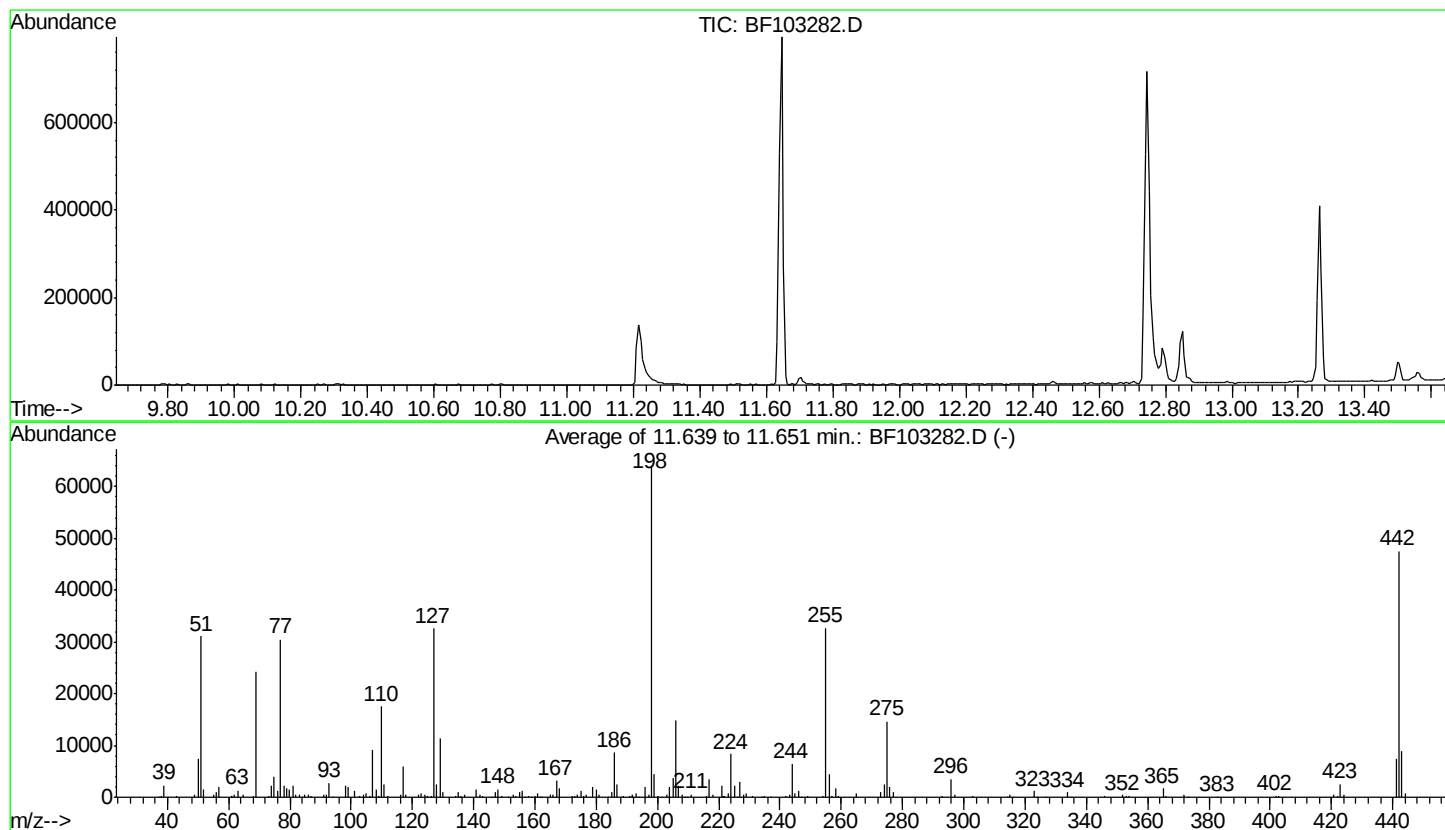

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.6	31109	PASS
68	69	0.00	2	1.4	352	PASS
69	198	0.00	100	38.0	24304	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	32531	PASS
197	198	0.00	2	0.7	466	PASS
198	198	100	100	100.0	64021	PASS
199	198	5	9	6.8	4347	PASS
275	198	10	60	22.9	14634	PASS
365	198	1	100	2.6	1651	PASS
441	443	0.01	100	83.5	7397	PASS
442	198	50	100	74.3	47549	PASS
443	442	15	24	18.6	8856	PASS