
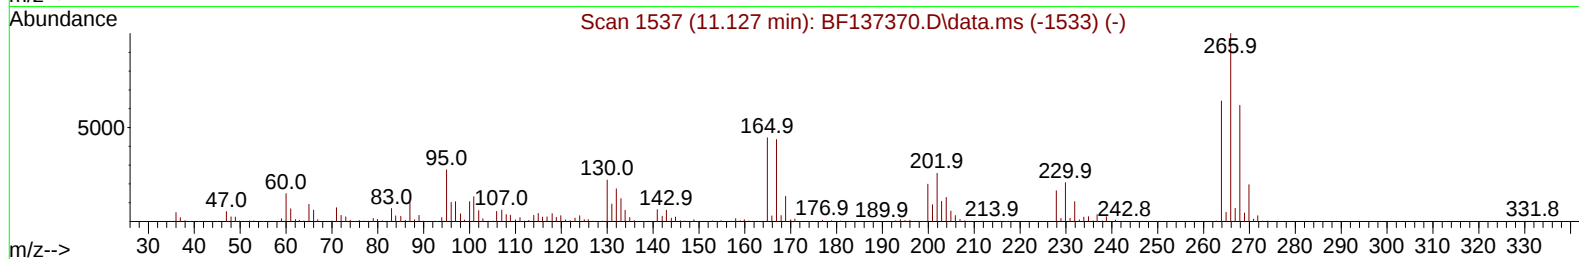
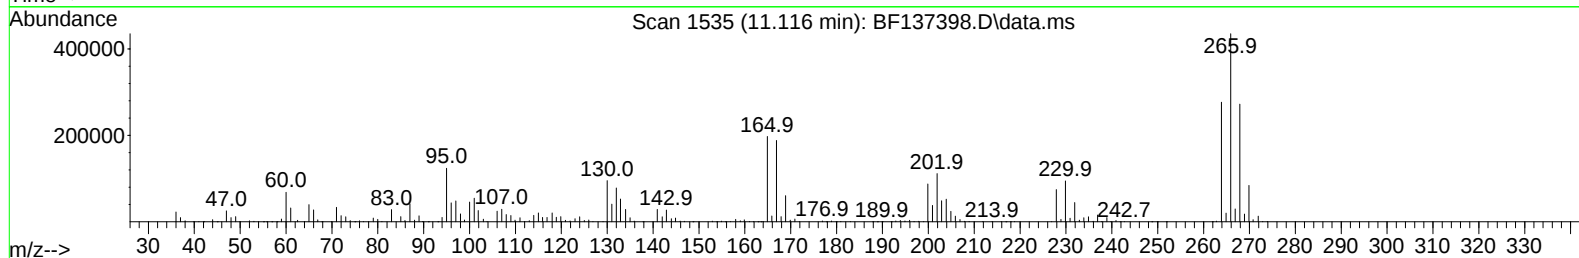


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022724\
Data File : BF137398.D
Acq On : 27 Feb 2024 11:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 12:06:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 04:23:49 2024
Response via : Initial Calibration

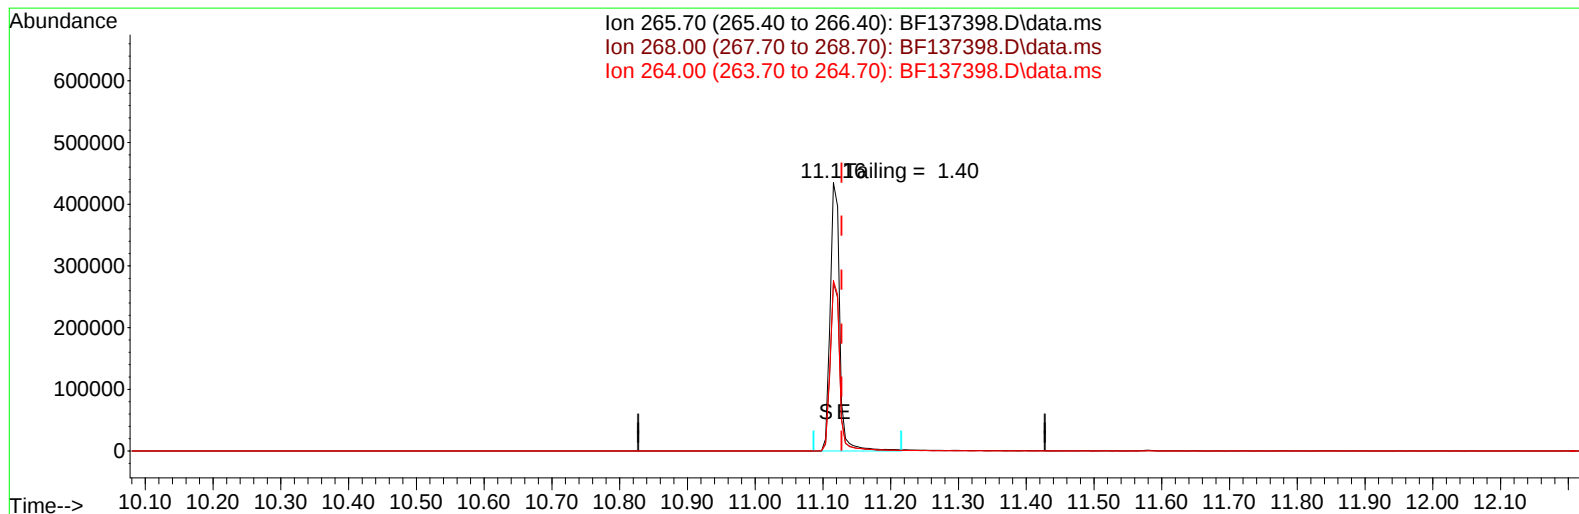

TIC: BF137398.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.012) 931772.19 ng

response 426740

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.80	62.59
264.00	64.10	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022724\
Data File : BF137398.D
Acq On : 27 Feb 2024 11:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 12:06:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 04:23:49 2024
Response via : Initial Calibration

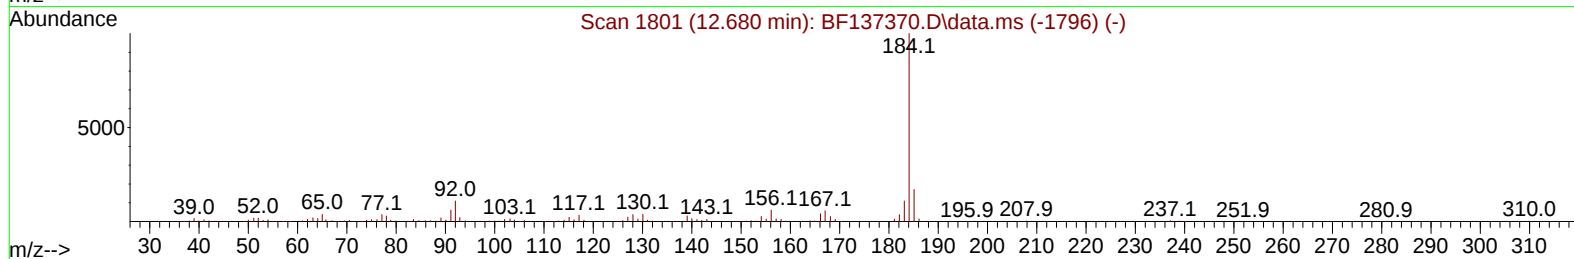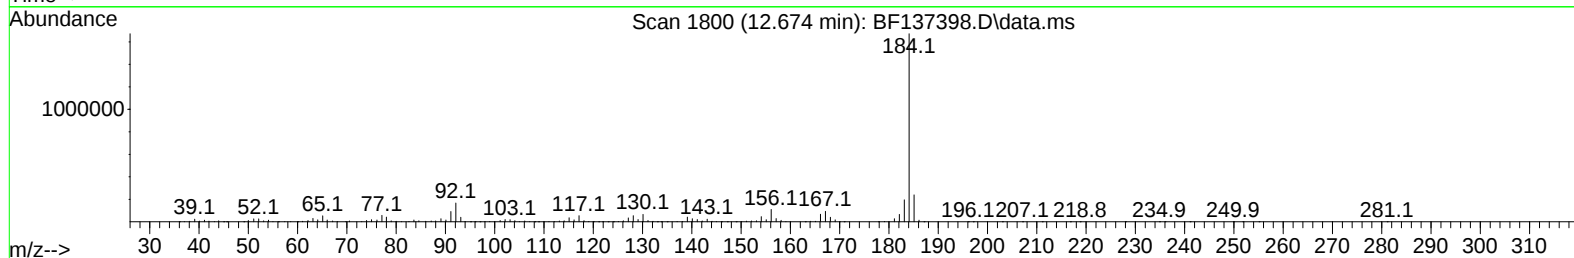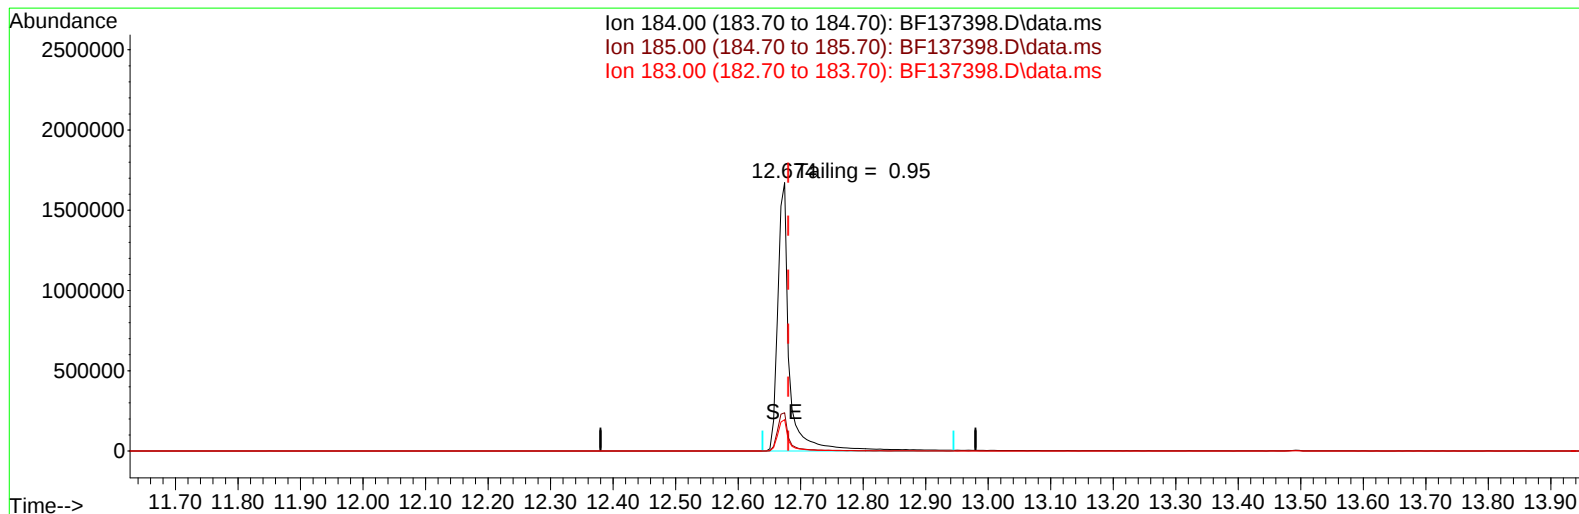

TIC: BF137398.D\data.ms

(77) Benzidine

12.674min (-0.006) 213243.78 ng m

response 2170448

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.10	14.29
183.00	11.00	11.68
0.00	0.00	0.00