
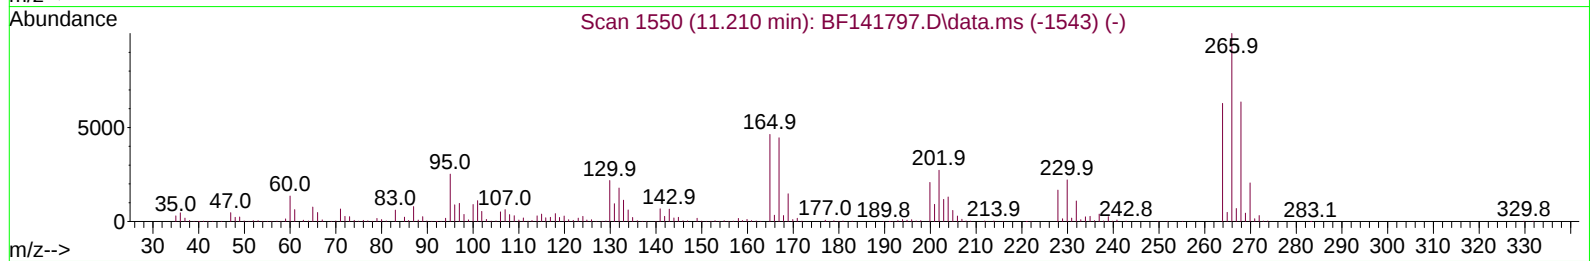
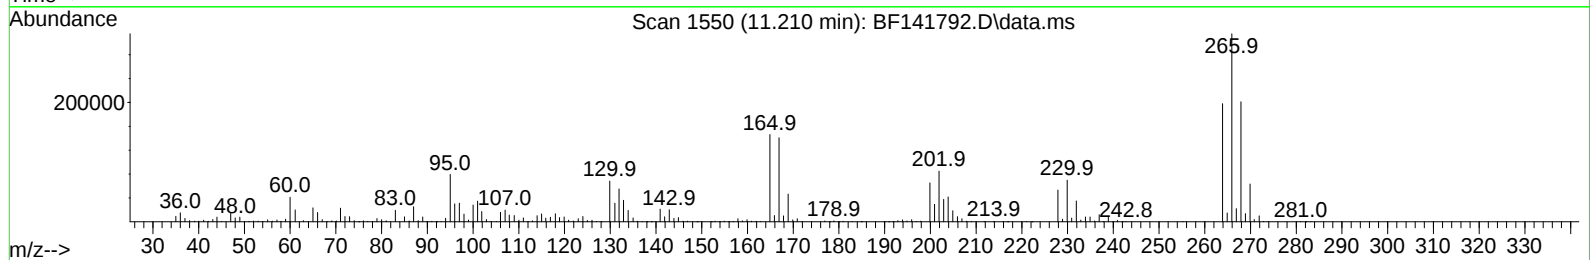


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022725\
Data File : BF141792.D
Acq On : 27 Feb 2025 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 01:59:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

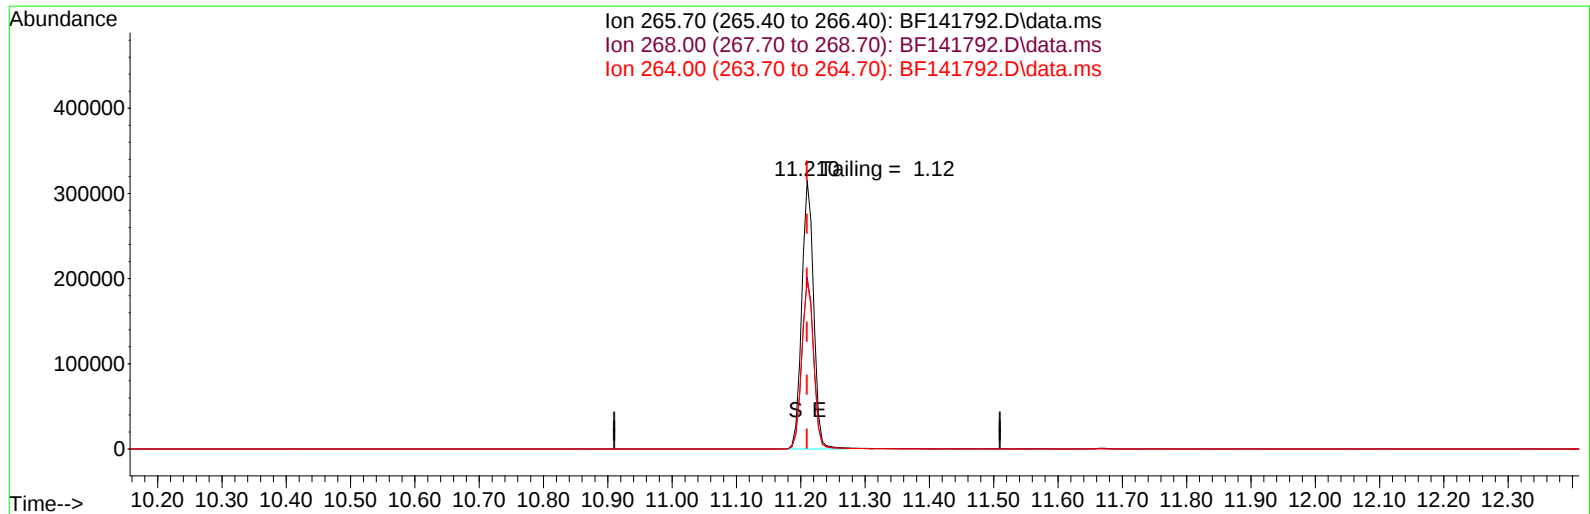

TIC: BF141792.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 55299.21 ng

response 409665

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.84
264.00	62.80	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022725\
Data File : BF141792.D
Acq On : 27 Feb 2025 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 01:59:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

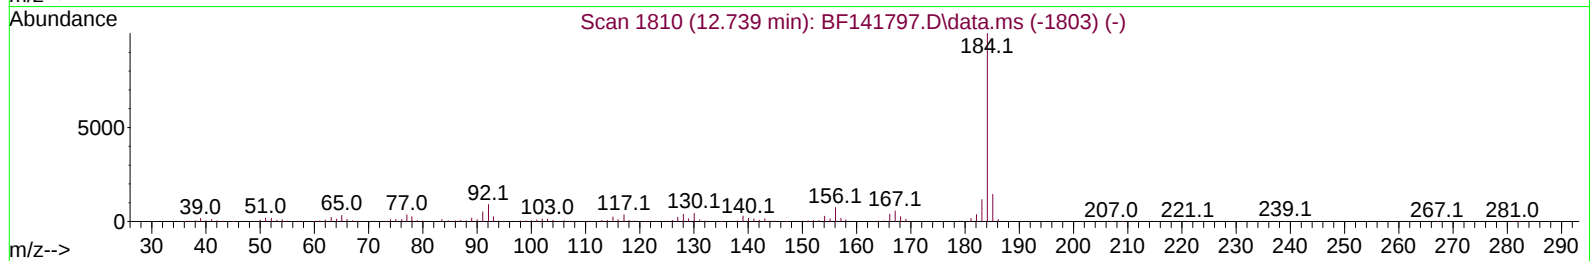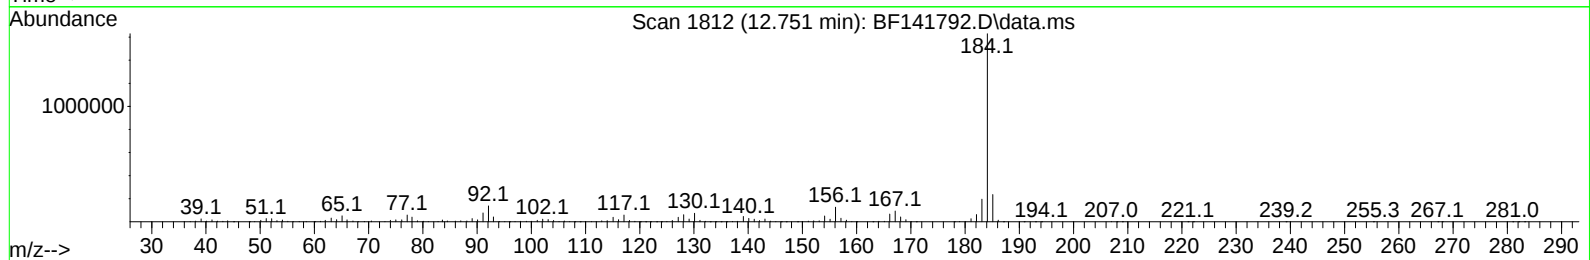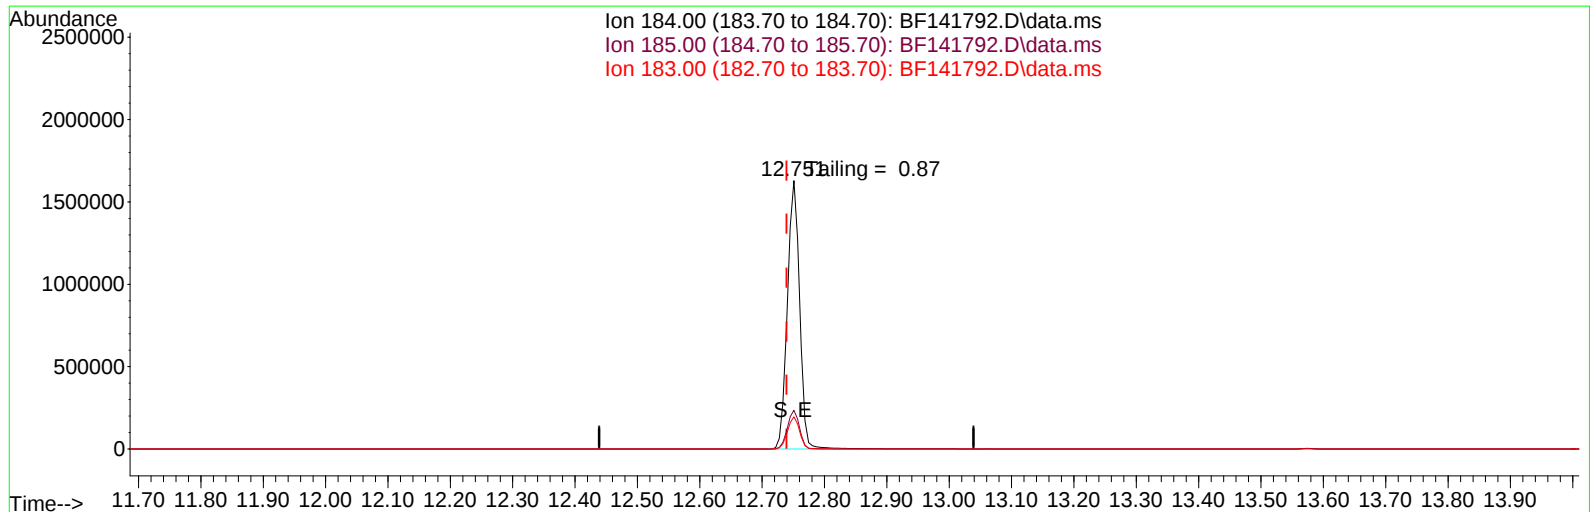

TIC: BF141792.D\data.ms

(77) Benzidine

12.751min (+ 0.012) 190021.56 ng

response 2231445

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.44
183.00	11.70	11.98
0.00	0.00	0.00