
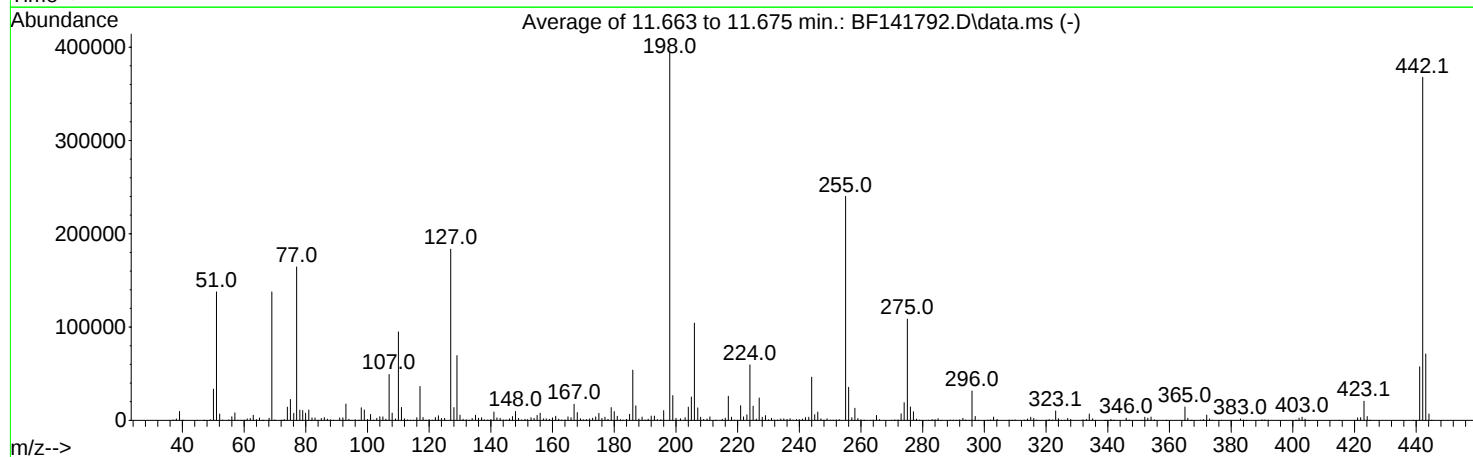


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022725\
Data File : BF141792.D
Acq On : 27 Feb 2025 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 28 01:48:16 2025

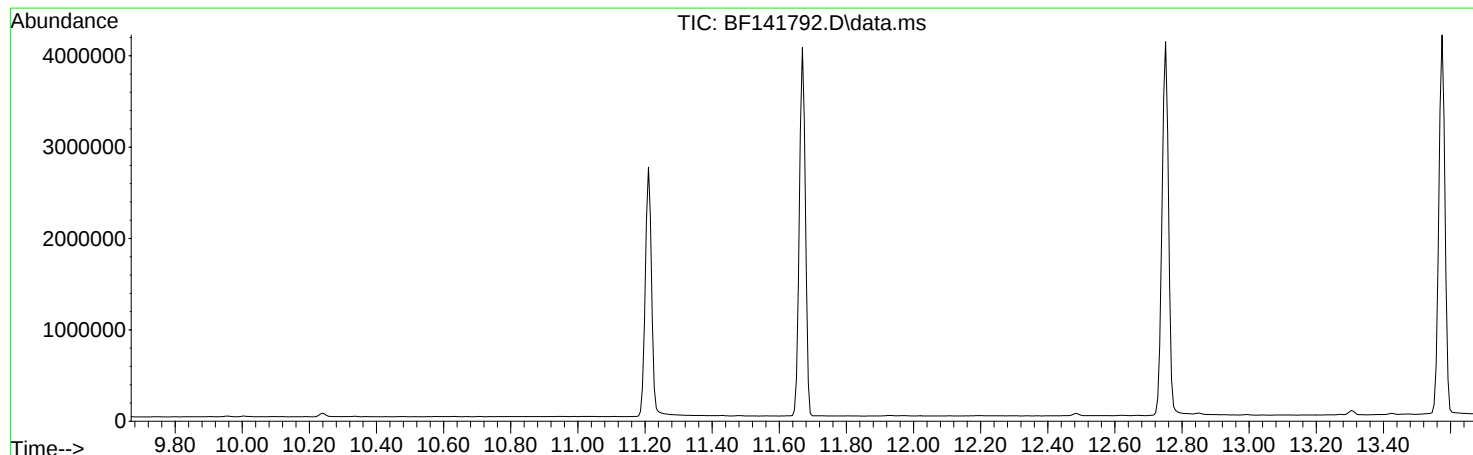

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	137699	PASS
68	69	0.00	2	1.7	2348	PASS
69	198	0.00	100	34.9	137773	PASS
70	69	0.00	2	0.4	593	PASS
127	198	10	80	46.5	183483	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	394304	PASS
199	198	5	9	6.7	26613	PASS
275	198	10	60	27.6	108637	PASS
365	198	1	100	3.7	14499	PASS
441	198	0.01	100	14.6	57517	PASS
442	442	50	100	100.0	367680	PASS
443	442	15	24	19.4	71267	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/27/2025	BNA_F	<u>BF141792.D</u>
Compound Name	Response	Retention Time
DDT	938485	13.575
DDD	9936	13.304
DDE	0	12.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9936	948421	1.05

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022725\
Data File : BF141792.D
Acq On : 27 Feb 2025 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 28 01:59:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

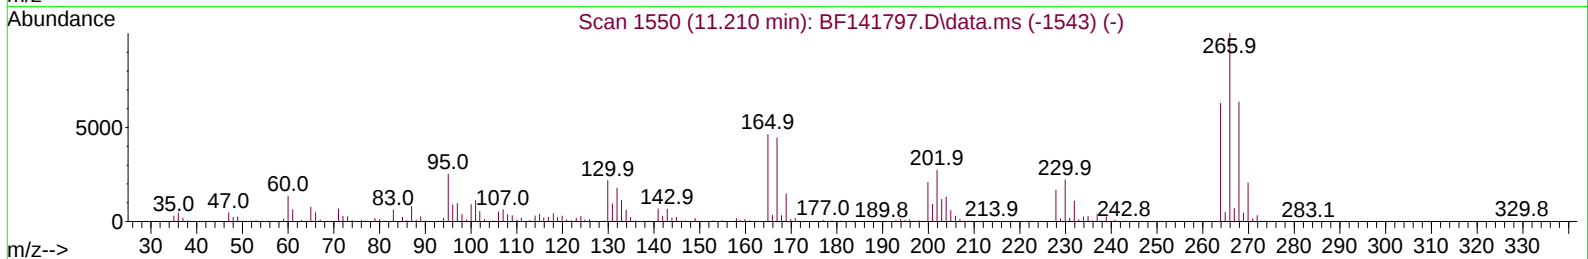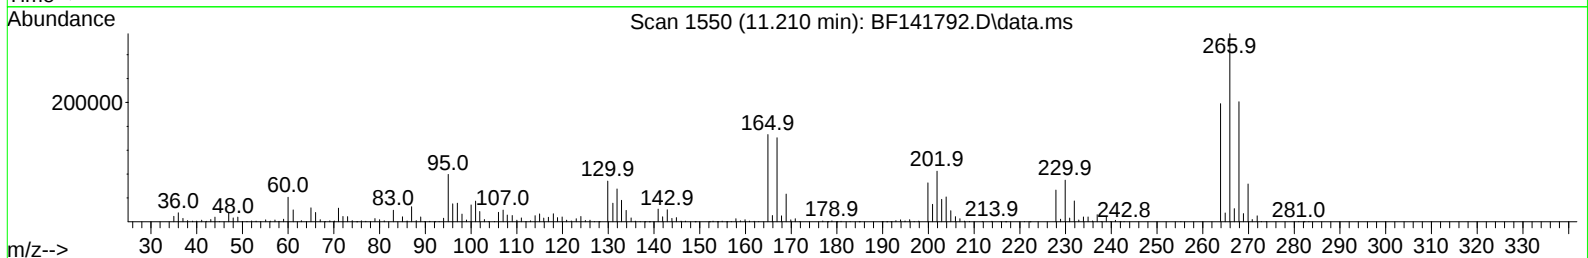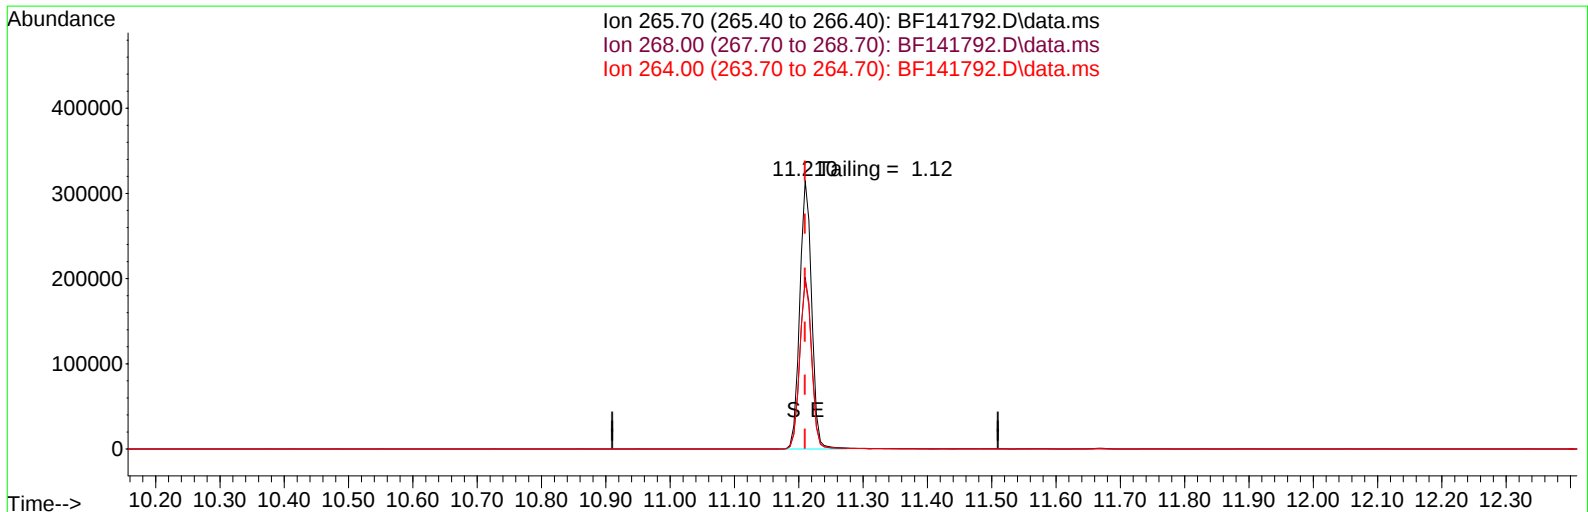

TIC: BF141792.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 55299.21 ng




response 409665

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.84
264.00	62.80	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022725\
Data File : BF141792.D
Acq On : 27 Feb 2025 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 28 01:59:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

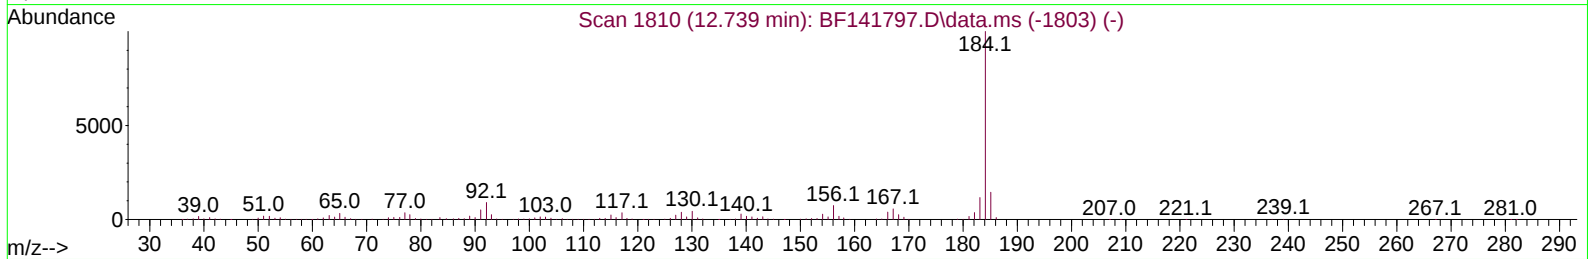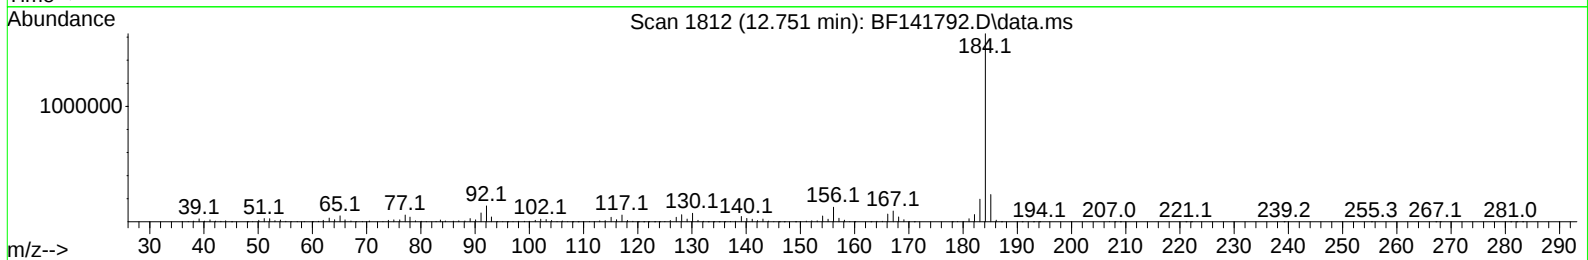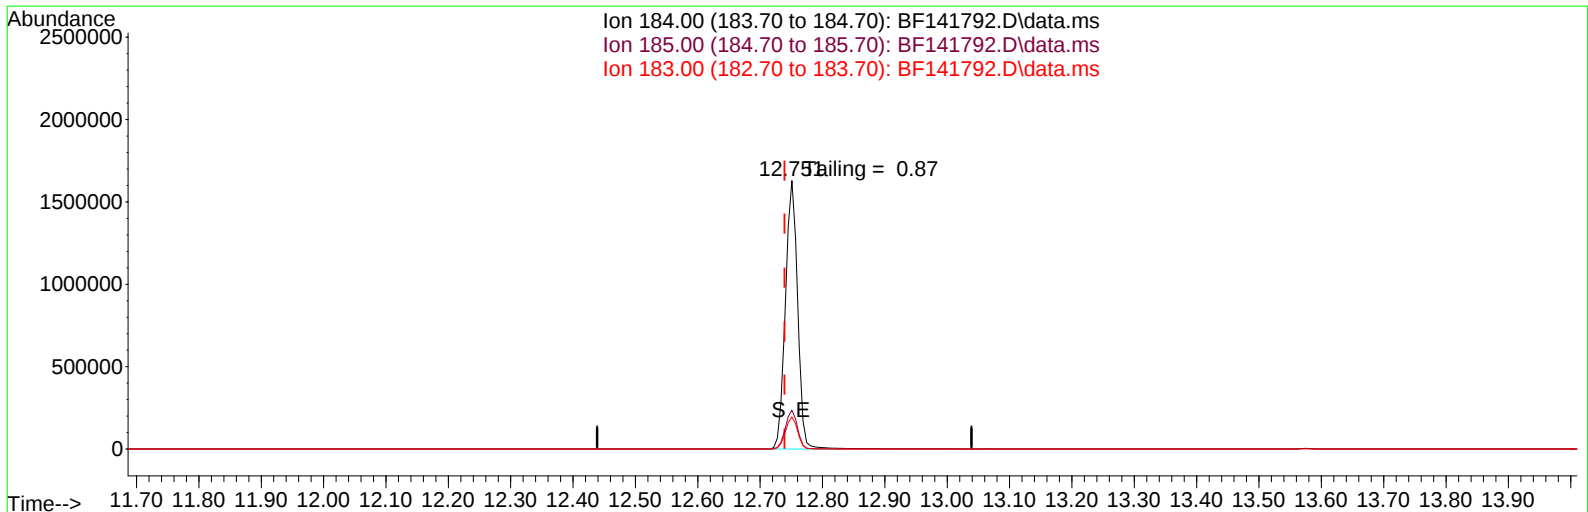

TIC: BF141792.D\data.ms

(77) Benzidine

12.751min (+ 0.012) 190021.56 ng

response 2231445

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.44
183.00	11.70	11.98
0.00	0.00	0.00