
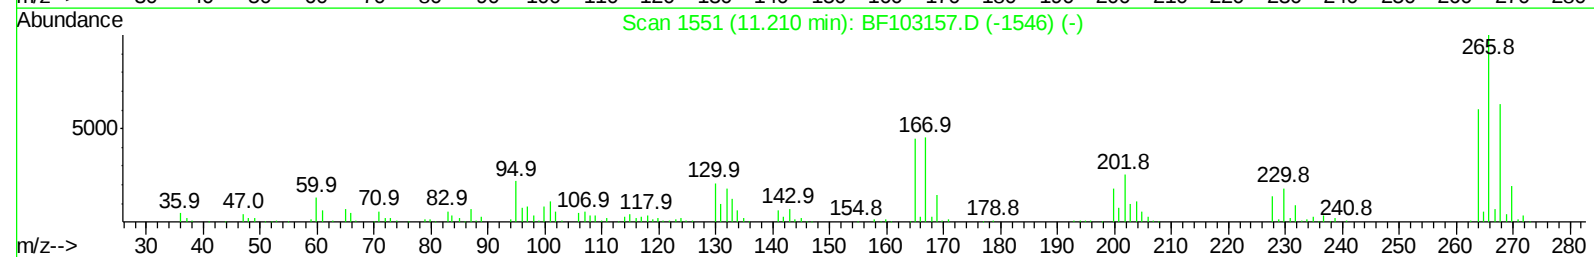
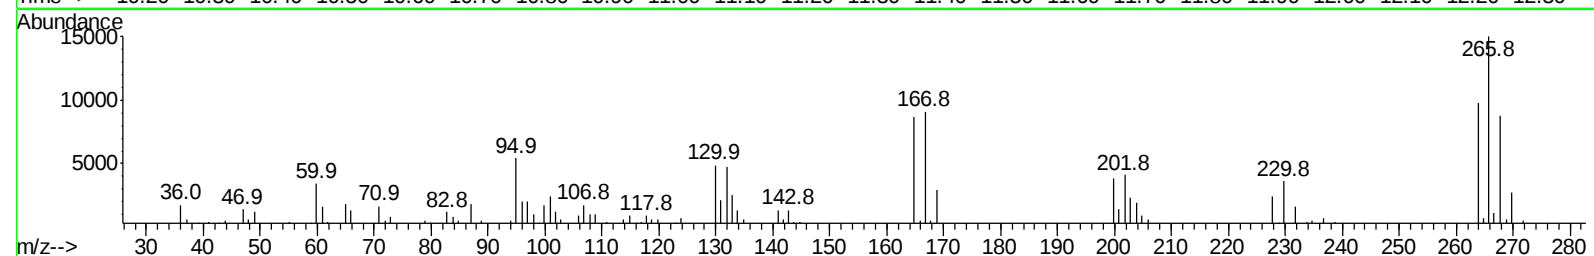


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF022818\
Data File : BF103318.D
Acq On : 1 Mar 2018 2:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 06:15:23 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 17:05:20 2018
Response via : Initial Calibration

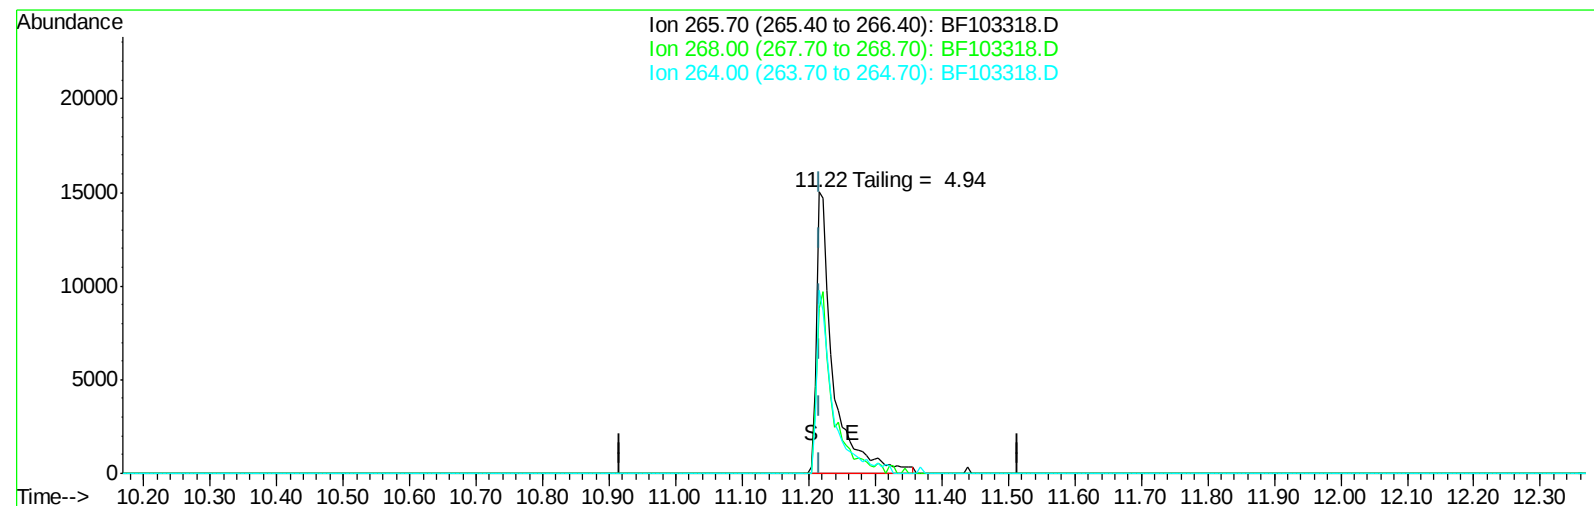

TIC: BF103318.D

(69) Pentachlorophenol (C)




11.216min (-0.000) 35800.70ng

response 26618

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.49
264.00	61.90	65.23
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF022818\
 Data File : BF103318.D
 Acq On : 1 Mar 2018 2:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 06:15:23 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 17:05:20 2018
 Response via : Initial Calibration

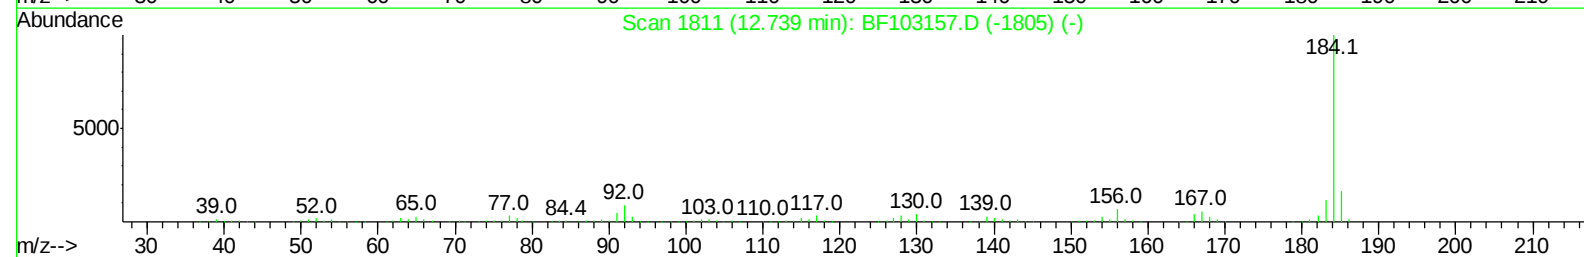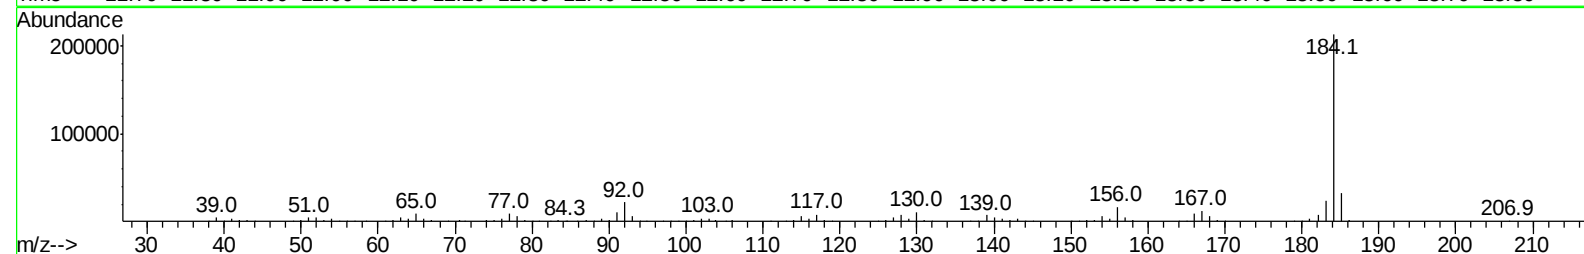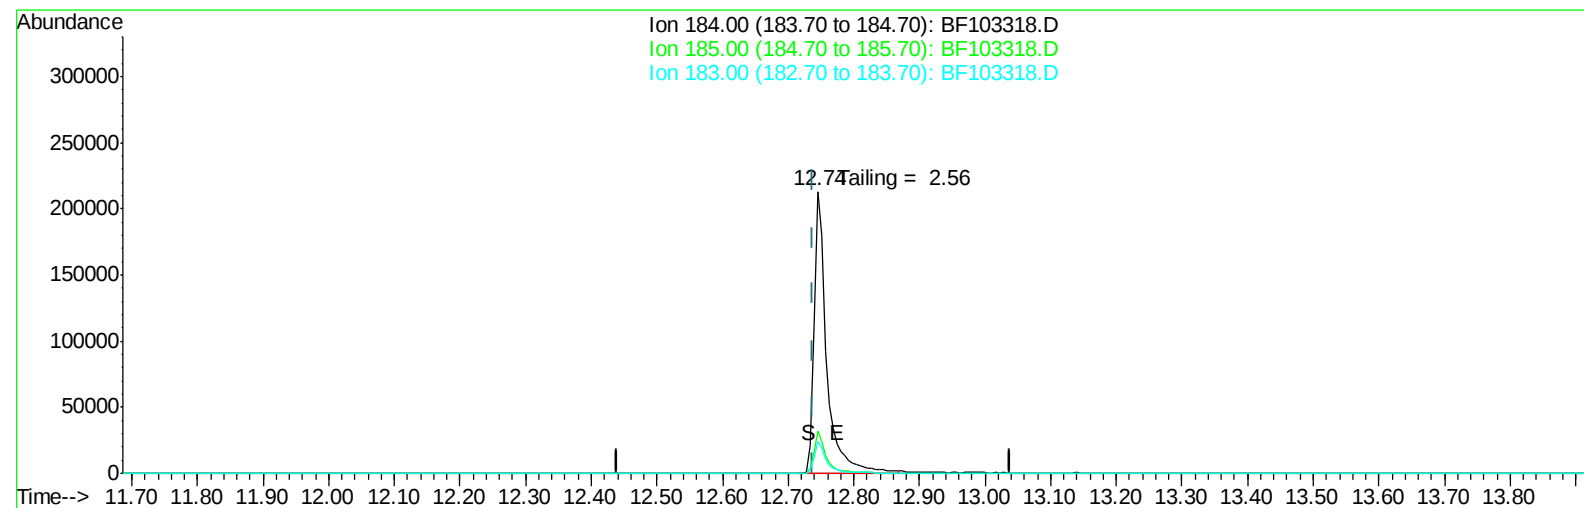

TIC: BF103318.D

(76) Benzidine

12.745min (+0.006) 0.00ng

response 290892

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.02
183.00	11.60	11.26
0.00	0.00	0.00