

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF022818\
 Data File : BF103321.D
 Acq On : 1 Mar 2018 4:17
 Operator : SJ/JU
 Sample : J1705-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 230KV-CONCRETE-REACTOR

Quant Time: Mar 01 06:04:22 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 17:05:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	154080	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	622125	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	241286	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	343301	20.00	ng	0.00
75) Chrysene-d12	14.06	240	274029	20.00	ng	0.00
86) Perylene-d12	15.55	264	206894	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	844123	82.86	ng	0.01
7) Phenol-d6	6.51	99	1122891	90.08	ng	0.00
23) Nitrobenzene-d5	7.44	82	782086	71.79	ng	0.00
41) 2,4,6-Tribromophenol	10.71	330	107217	52.50	ng	0.00
44) 2-Fluorobiphenyl	9.23	172	1130900	79.49	ng	0.00
78) Terphenyl-d14	12.99	244	762967	66.93	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.63	163	91860	4.746	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF022818\
Data File : BF103321.D
Acq On : 1 Mar 2018 4:17
Operator : SJ/JU
Sample : J1705-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
230KV-CONCRETE-REACTOR

Quant Time: Mar 01 06:04:22 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 17:05:20 2018
Response via : Initial Calibration

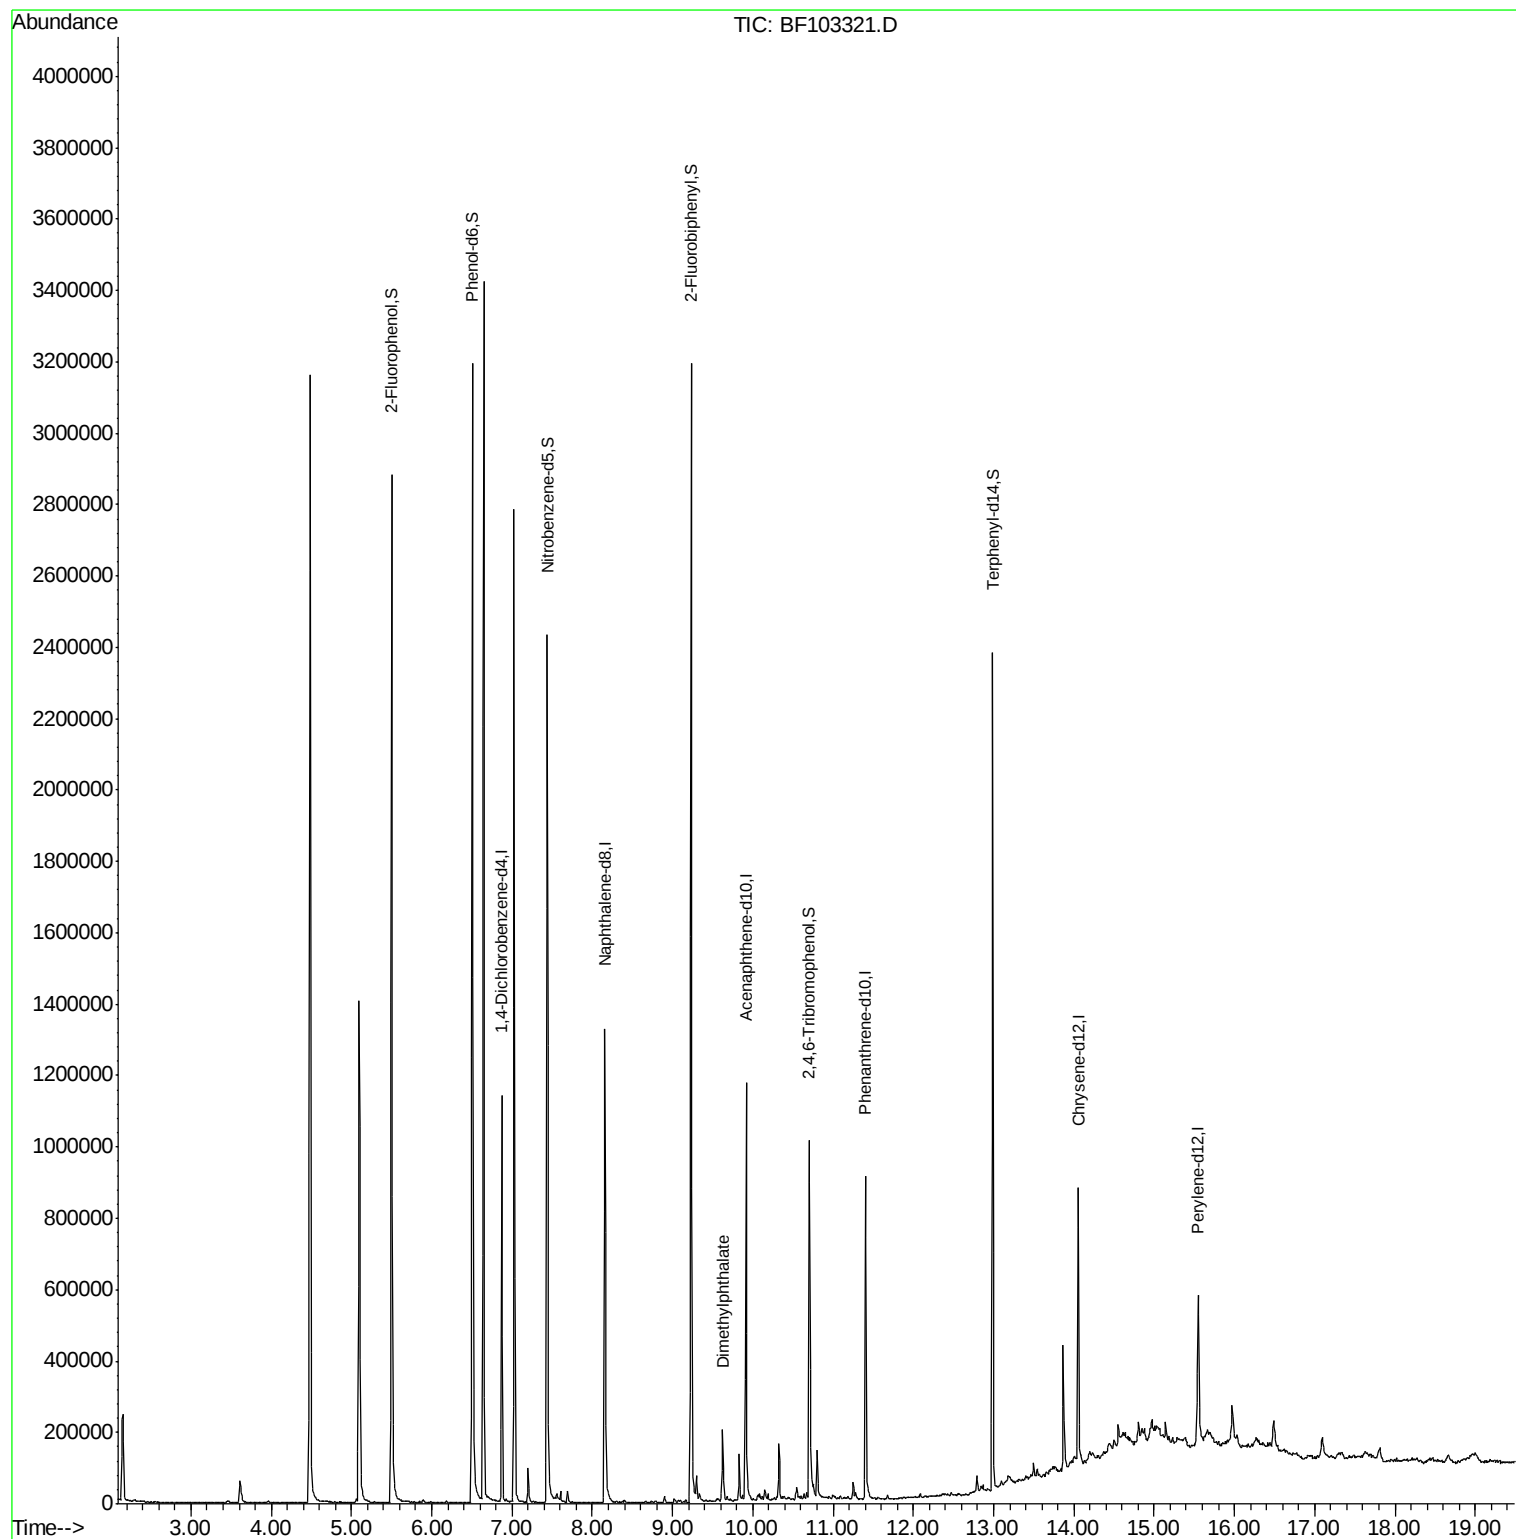




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.87 min Scan# 814
Delta R.T. -0.00 min
Lab File: BF103321.D
Acq: 1 Mar 2018 4:17

Instrument :
BNA_F
ClientSampleId :
230KV-CONCRETE-REACTOR

Tot Ion:152 Resp: 154080
Ion Ratio Lower Upper
152 100
150 152.1 124.6 186.8
115 63.6 50.1 75.1

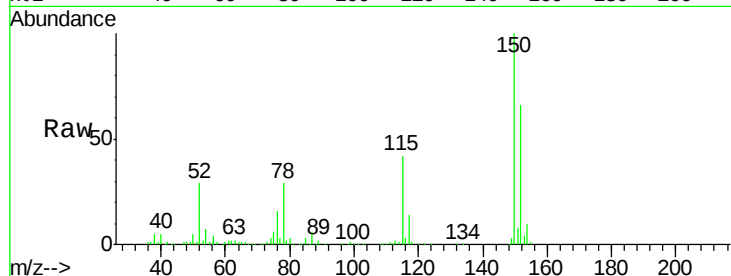


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

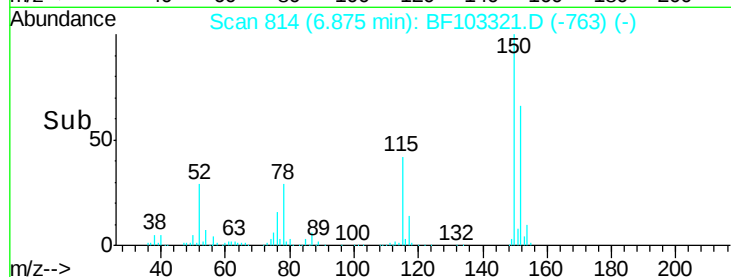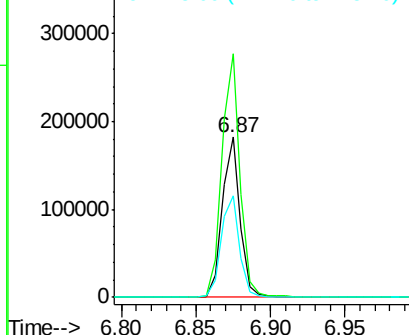



#5


2-Fluorophenol
Concen: 82.858 ng
RT: 5.50 min Scan# 581
Delta R.T. 0.01 min
Lab File: BF103321.D
Acq: 1 Mar 2018 4:17

Tgt Ion:112 Resp: 844123
Ion Ratio Lower Upper
112 100
64 63.4 47.9 71.9
63 33.3 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

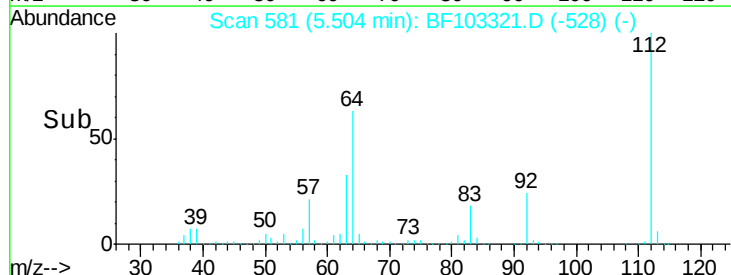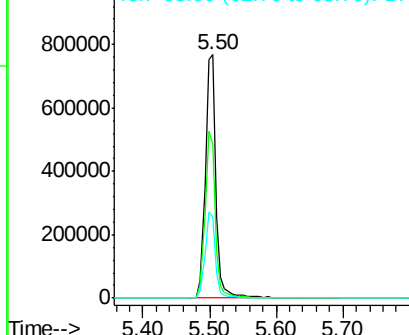

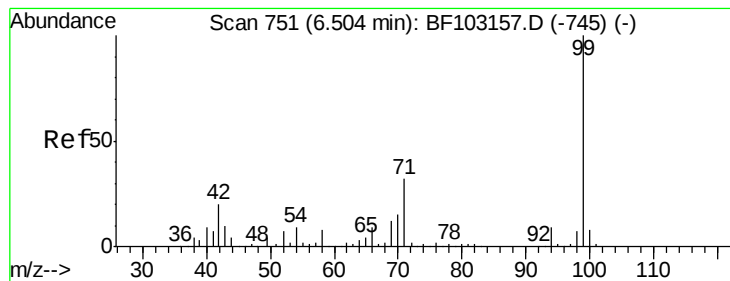

#7

Phenol-d6

Concen: 90.076 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.00 min

Lab File: BF103321.D

Acq: 1 Mar 2018 4:17

Instrument :


BNA_F

ClientSampleId :

230KV-CONCRETE-REACTOR

Tot Ion: 99 Resp: 1122891

Ion	Ratio	Lower	Upper
99	100		
42	21.4	14.5	21.7
71	33.5	25.4	38.0


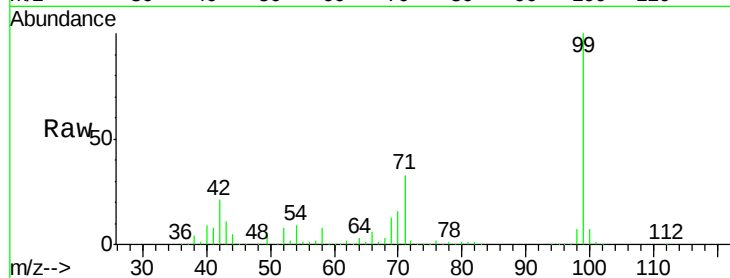


Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

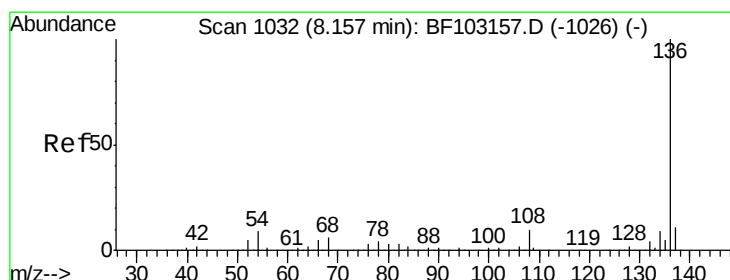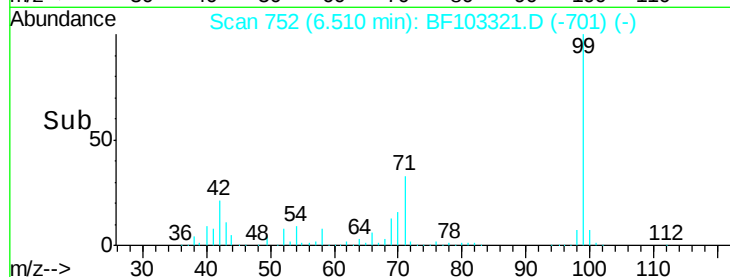

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1032



Delta R.T. -0.00 min


Lab File: BF103321.D

Acq: 1 Mar 2018 4:17

Tgt Ion:136 Resp: 622125

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.9	13.3
54	9.5	6.6	9.8
68	6.9	5.0	7.4

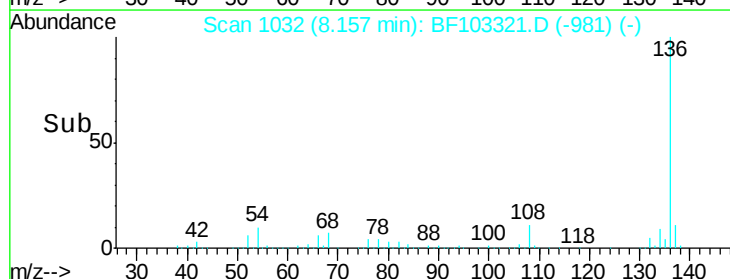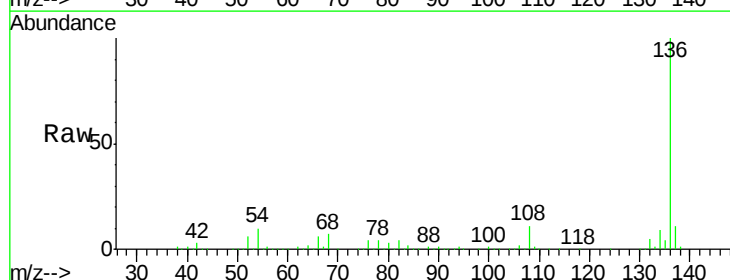


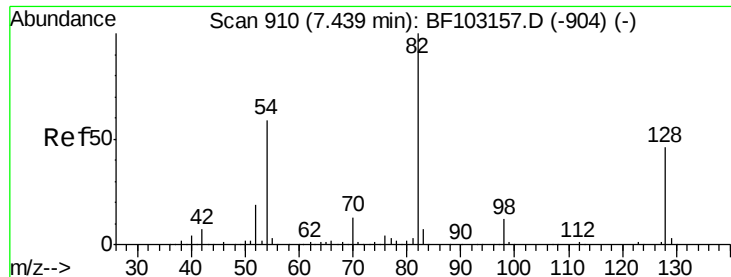




#23
Nitrobenzene-d5
Concen: 71.792 ng
RT: 7.44 min Scan# 910
Delta R.T. -0.01 min
Lab File: BF103321.D
Acq: 1 Mar 2018 4:17

Instrument :
BNA_F
ClientSampleId :
230KV-CONCRETE-REACTOR

Tot Ion: 82 Resp: 782086
Ion Ratio Lower Upper
82 100
128 44.2 36.1 54.1
54 63.7 41.4 62.2#

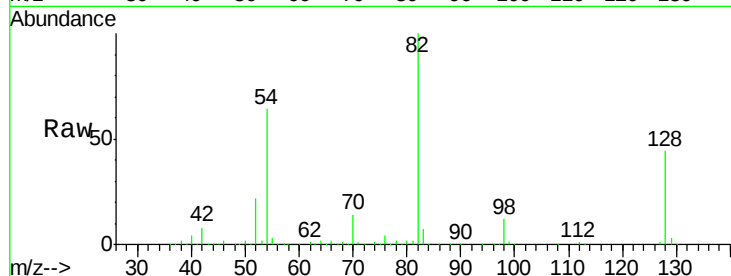


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

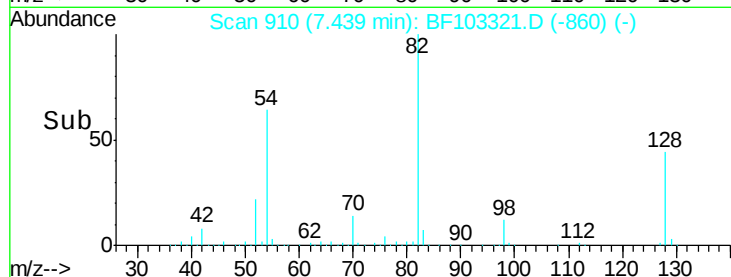
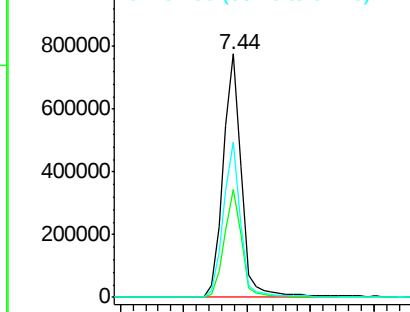


#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.92 min Scan# 1331
Delta R.T. -0.00 min
Lab File: BF103321.D
Acq: 1 Mar 2018 4:17

Tgt Ion:164 Resp: 241286
Ion Ratio Lower Upper
164 100
162 103.5 86.1 129.1
160 46.9 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

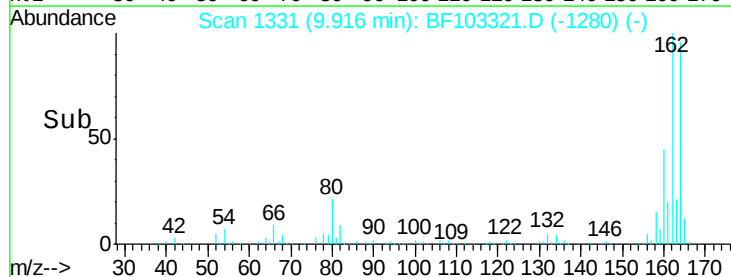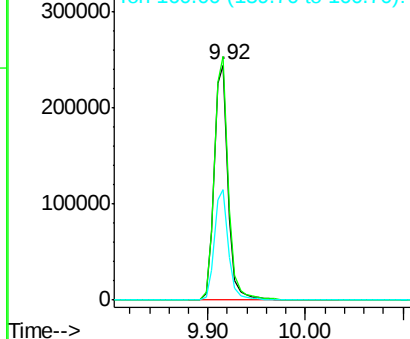







#41
 2,4,6-Tribromophenol
 Concen: 52.497 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.00 min
 Lab File: BF103321.D
 Acq: 1 Mar 2018 4:17

Instrument :
 BNA_F
 ClientSampleId :
 230KV-CONCRETE-REACTOR

Tot Ion:330 Resp: 107217
 Ion Ratio Lower Upper
 330 100
 332 103.5 77.0 115.6
 141 50.3 29.9 44.9#

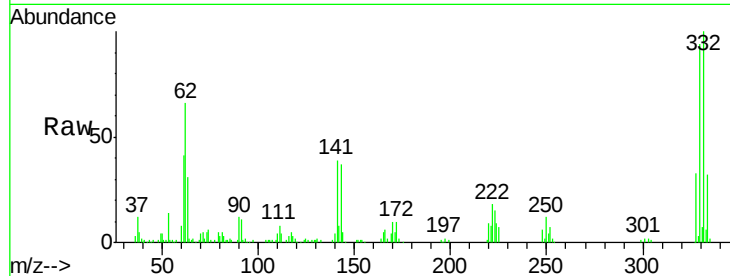


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

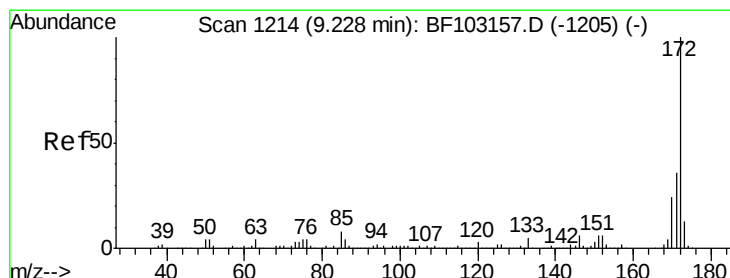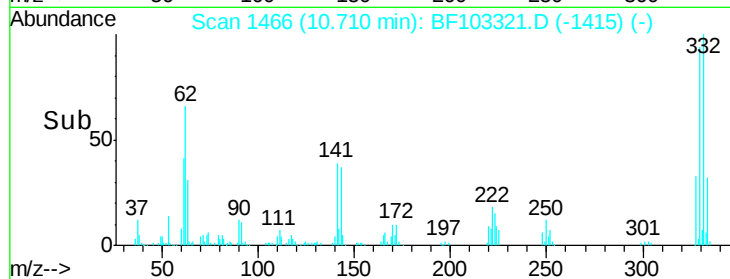
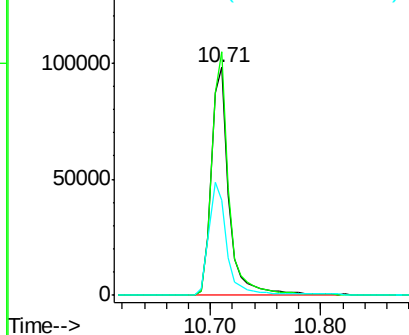



#44
 2-Fluorobiphenyl
 Concen: 79.493 ng
 RT: 9.23 min Scan# 1215
 Delta R.T. -0.00 min
 Lab File: BF103321.D
 Acq: 1 Mar 2018 4:17

Tgt Ion:172 Resp: 1130900
 Ion Ratio Lower Upper
 172 100
 171 35.3 29.7 44.5
 170 24.7 19.6 29.4

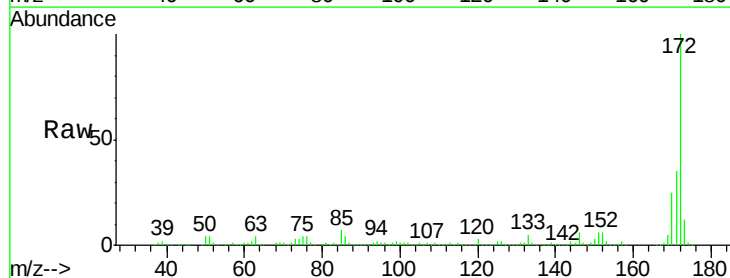

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

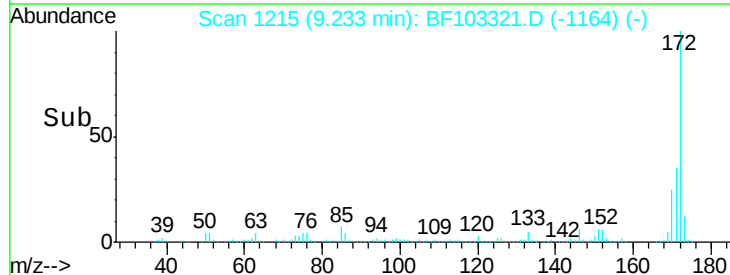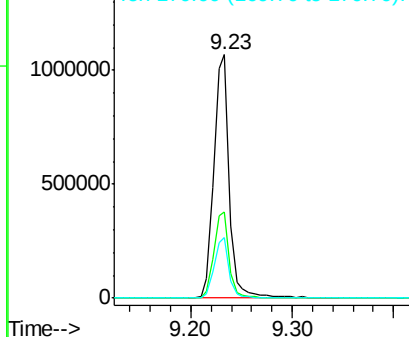

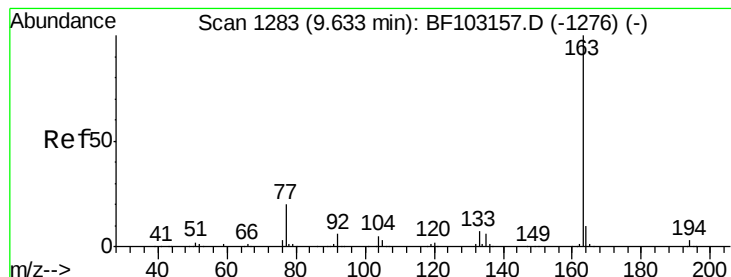

#49

Dimethylphthalate

Concen: 4.746 ng

RT: 9.63 min Scan# 1282

Delta R.T. -0.01 min

Lab File: BF103321.D

Acq: 1 Mar 2018 4:17

Instrument :

BNA_F

ClientSampleId :

230KV-CONCRETE-REACTOR


Tot Ion:163 Resp: 91860

Ion Ratio Lower Upper

163 100

194 3.3 2.7 4.1




164 9.5 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

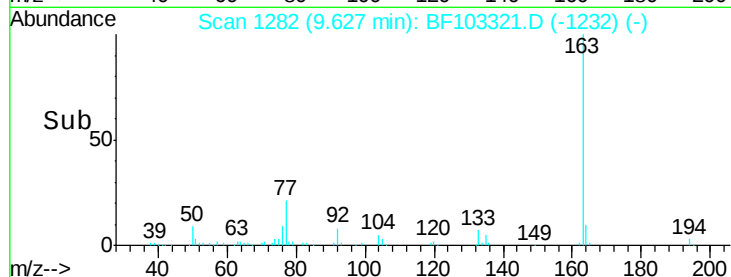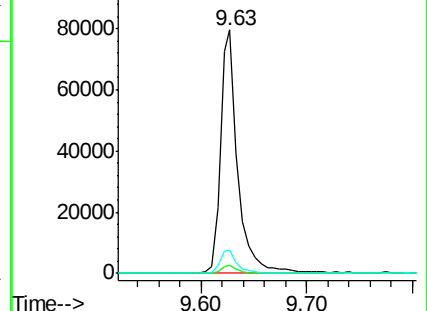

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.40 min Scan# 1584

Delta R.T. -0.00 min

Lab File: BF103321.D

Acq: 1 Mar 2018 4:17


Tgt Ion:188 Resp: 343301

Ion Ratio Lower Upper

188 100

94 12.0 8.5 12.7



80 14.0 9.2 13.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

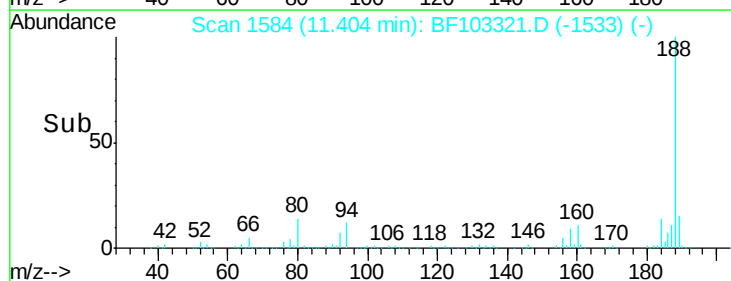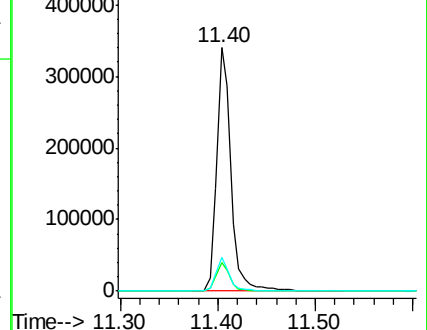

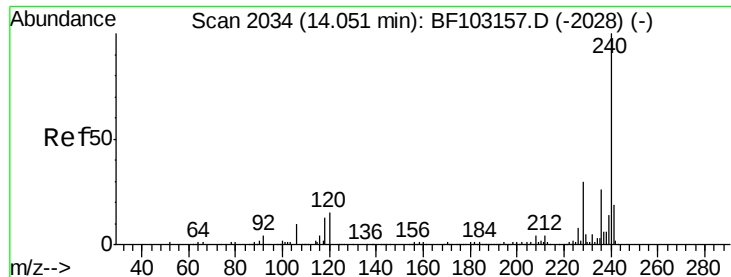

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.06 min Scan# 2035

Delta R.T. -0.00 min

Lab File: BF103321.D

Acq: 1 Mar 2018 4:17

Instrument :

BNA_F

ClientSampleId :

230KV-CONCRETE-REACTOR


Tot Ion:240 Resp: 274029

Ion Ratio Lower Upper

240 100

120 14.8 9.5 14.3#




236 27.3 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

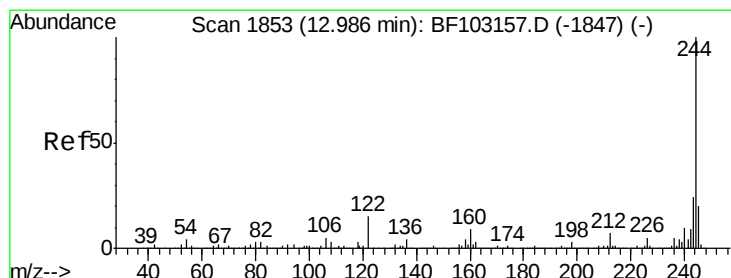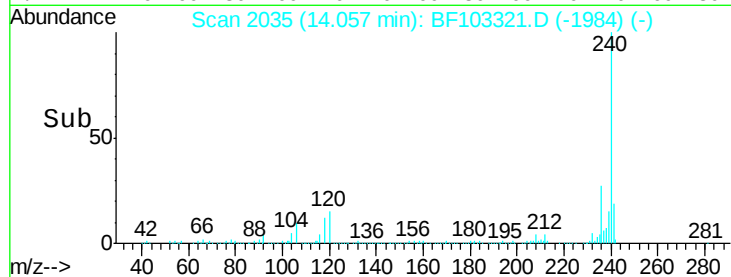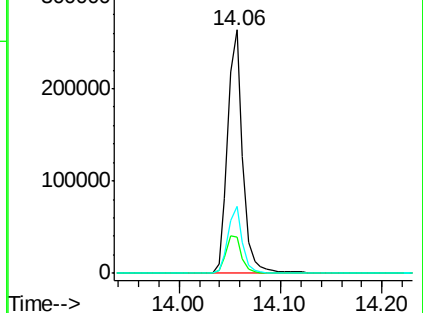

#78

Terphenyl-d14

Concen: 66.930 ng

RT: 12.99 min Scan# 1854

Delta R.T. -0.00 min

Lab File: BF103321.D

Acq: 1 Mar 2018 4:17


Tgt Ion:244 Resp: 762967

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0



122 12.9 11.0 16.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

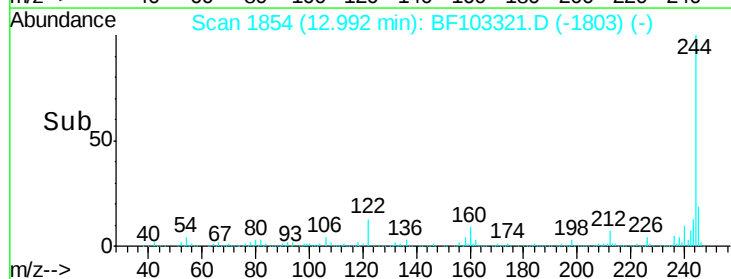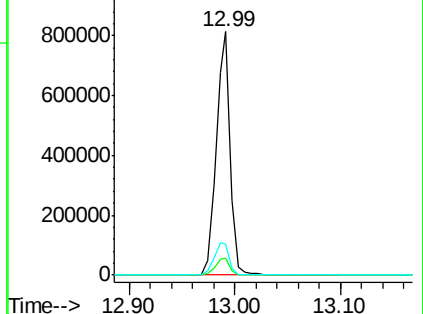


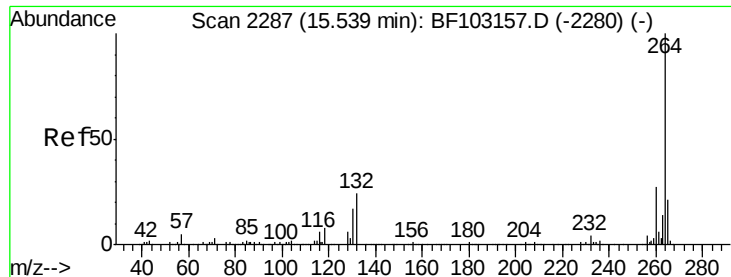

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.55 min Scan# 2289
Delta R.T. -0.01 min
Lab File: BF103321.D
Acq: 1 Mar 2018 4:17

Instrument :
BNA_F
ClientSampleId :
230KV-CONCRETE-REACTOR

Tot Ion:264 Resp: 206894
Ion Ratio Lower Upper
264 100
260 23.6 19.2 28.8
265 20.2 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

