

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA\_F\DATA\BF022818\  
 Data File : BF103303.D  
 Acq On : 28 Feb 2018 19:51  
 Operator : SJ/JU  
 Sample : J1709-01 50X  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DRUM-1-2

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF022218.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.504       | 578           | 581         | 592          | rBV      | 36576          | 65532         | 5.07%           | 0.941%        |
| 2         | 6.522       | 751           | 754         | 766          | rBV4     | 28619          | 70211         | 5.43%           | 1.008%        |
| 3         | 6.651       | 772           | 776         | 781          | rBV      | 57458          | 72605         | 5.62%           | 1.043%        |
| 4         | 6.692       | 781           | 783         | 787          | rVB2     | 14957          | 13528         | 1.05%           | 0.194%        |
| 5         | 6.869       | 810           | 813         | 824          | rBV      | 904882         | 958993        | 74.18%          | 13.771%       |
| 6         | 7.028       | 836           | 840         | 849          | rBV      | 56328          | 60816         | 4.70%           | 0.873%        |
| 7         | 7.445       | 907           | 911         | 922          | rBV      | 26852          | 51977         | 4.02%           | 0.746%        |
| 8         | 8.157       | 1028          | 1032        | 1047         | rBV      | 1264887        | 1292831       | 100.00%         | 18.565%       |
| 9         | 9.233       | 1212          | 1215        | 1223         | rBV      | 47579          | 57872         | 4.48%           | 0.831%        |
| 10        | 9.916       | 1327          | 1331        | 1347         | rVB      | 1137342        | 1245221       | 96.32%          | 17.881%       |
| 11        | 10.469      | 1422          | 1425        | 1429         | rVB      | 12860          | 13799         | 1.07%           | 0.198%        |
| 12        | 10.716      | 1462          | 1467        | 1473         | rBV3     | 20091          | 26266         | 2.03%           | 0.377%        |
| 13        | 11.404      | 1580          | 1584        | 1595         | rBV      | 1022355        | 1087382       | 84.11%          | 15.615%       |
| 14        | 11.486      | 1595          | 1598        | 1603         | rVB      | 19605          | 21314         | 1.65%           | 0.306%        |
| 15        | 11.939      | 1673          | 1675        | 1681         | rBV2     | 10917          | 13278         | 1.03%           | 0.191%        |
| 16        | 12.027      | 1686          | 1690        | 1692         | rBV2     | 14146          | 18183         | 1.41%           | 0.261%        |
| 17        | 12.621      | 1788          | 1791        | 1795         | rBV      | 88250          | 90315         | 6.99%           | 1.297%        |
| 18        | 12.851      | 1825          | 1830        | 1838         | rBV      | 76338          | 97833         | 7.57%           | 1.405%        |
| 19        | 12.986      | 1849          | 1853        | 1856         | rBV      | 45293          | 46152         | 3.57%           | 0.663%        |
| 20        | 13.180      | 1884          | 1886        | 1893         | rVB7     | 11195          | 14123         | 1.09%           | 0.203%        |
| 21        | 13.839      | 1995          | 1998        | 2002         | rBV2     | 22129          | 29184         | 2.26%           | 0.419%        |
| 22        | 14.051      | 2029          | 2034        | 2045         | rBV      | 716646         | 863619        | 66.80%          | 12.401%       |
| 23        | 15.556      | 2285          | 2290        | 2300         | rVB      | 531605         | 752856        | 58.23%          | 10.811%       |


Sum of corrected areas: 6963890

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF022818\  
Data File : BF103303.D  
Acq On : 28 Feb 2018 19:51  
Operator : SJ/JU  
Sample : J1709-01 50X  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DRUM-1-2

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF022218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

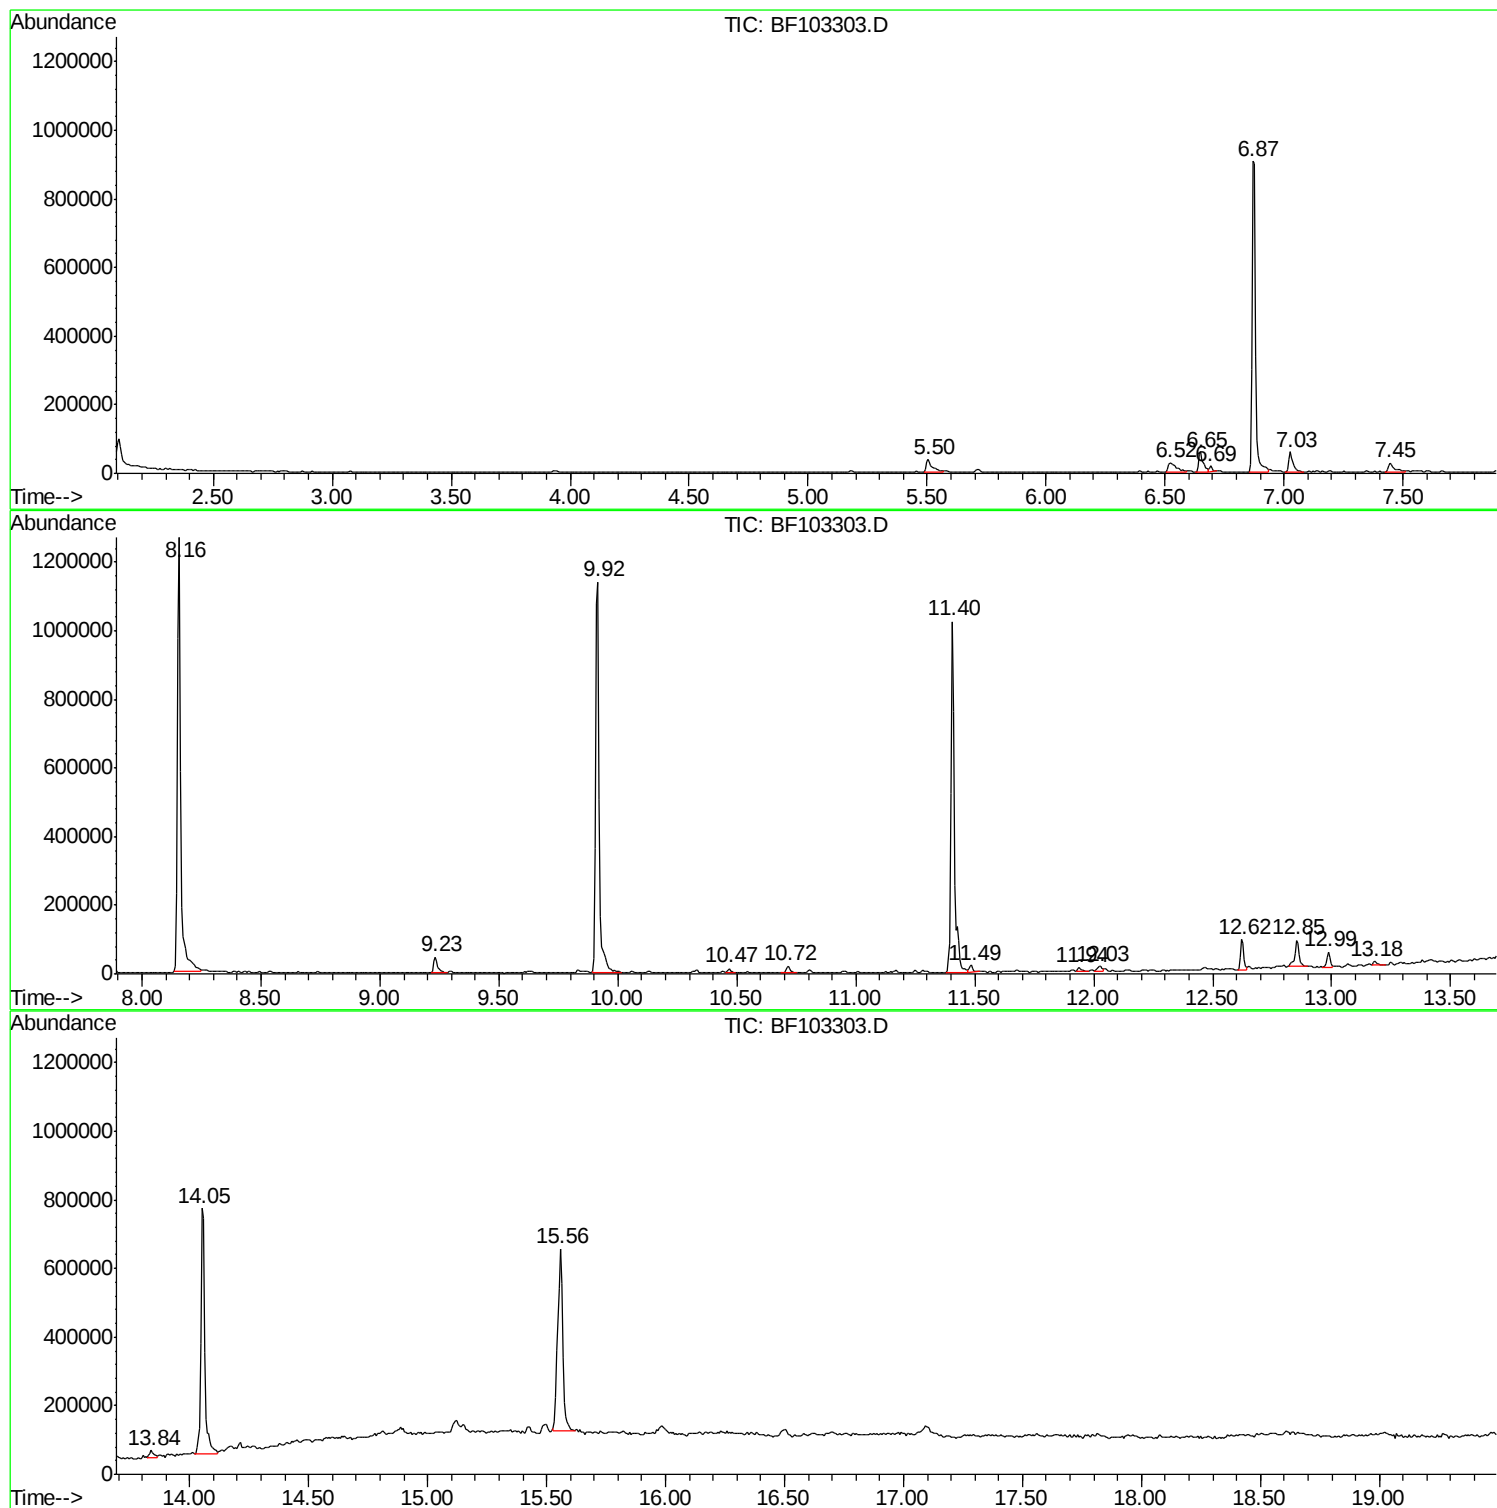

Data\_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA\_F\DATA\BF022818\  
Data\_File : BF103303.D  
Acq\_On : 28\_Feb\_2018\_ 19:511  
Operator : SJ/JUU  
Sample : J1709-01\_50XX  
Misc :  
ALS\_Vial : 11 Sample\_Multiplier: 11

Instrument :  
BNA\_F  
ClientSampleId :  
DRUM-1-2

Quant\_Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF022218.MM  
Quant\_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC\_Library : C:\DATABASE\NIST11.LL  
TIC\_Integration Parameters: LSCINT.PP

| TIC Top Hit name | RT | EstConc | Units | Response | Internal Standard |
|------------------|----|---------|-------|----------|-------------------|
|                  |    |         |       | #        | RT Resp Conc      |

No Library Search Compounds Detected

\*\*\*\*\*