


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF022818\
 Data File : BF103293.D
 Acq On : 28 Feb 2018 14:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 27 17:05:20 2018

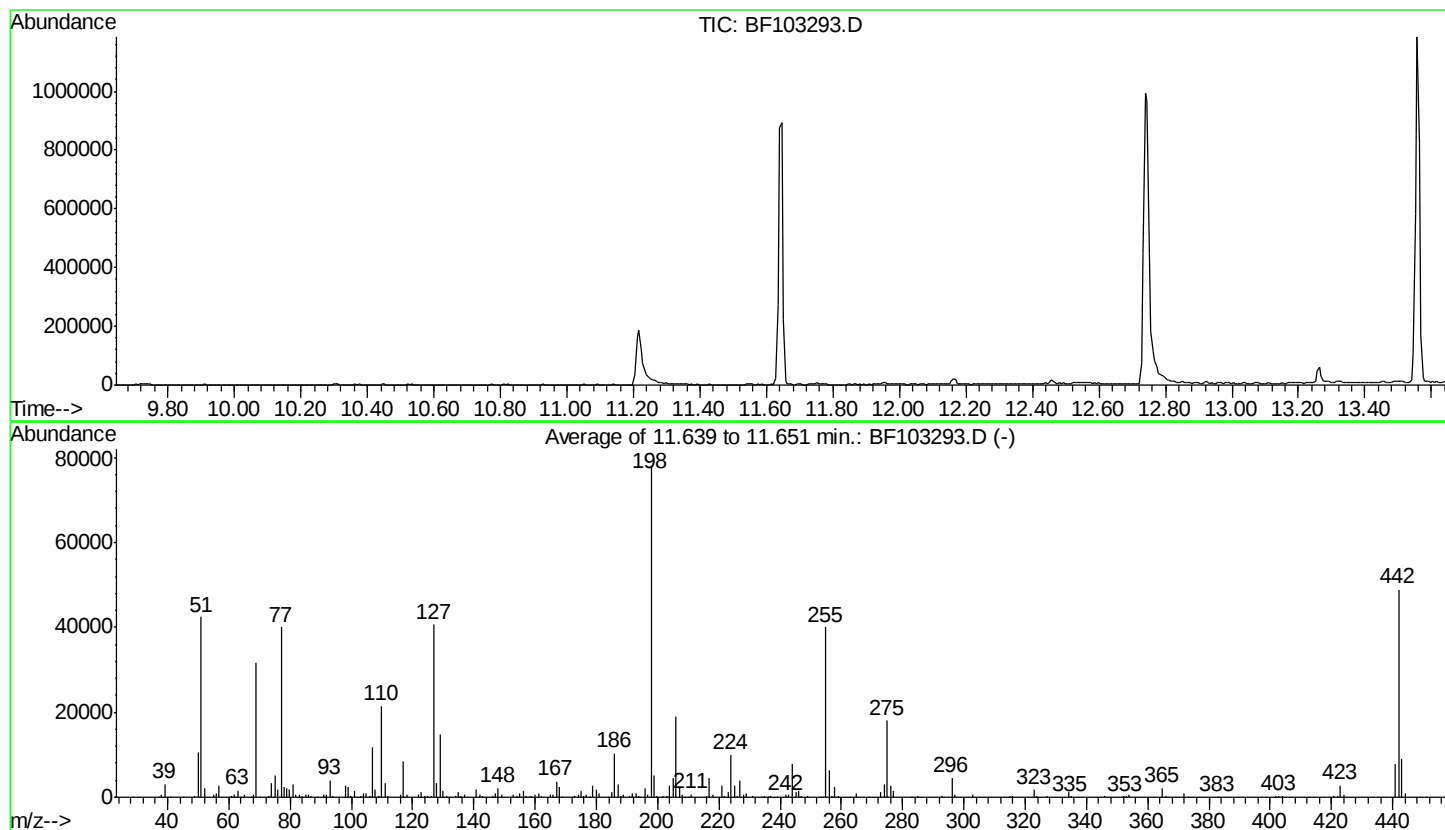

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	42376	PASS
68	69	0.00	2	1.7	552	PASS
69	198	0.00	100	40.5	31647	PASS
70	69	0.00	2	0.4	125	PASS
127	198	10	80	52.1	40686	PASS
197	198	0.00	2	0.7	546	PASS
198	198	100	100	100.0	78088	PASS
199	198	5	9	6.7	5255	PASS
275	198	10	60	23.1	18050	PASS
365	198	1	100	2.7	2130	PASS
441	443	0.01	100	86.6	7846	PASS
442	198	50	100	62.6	48848	PASS
443	442	15	24	18.5	9056	PASS