


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF022818\
 Data File : BF103318.D
 Acq On : 1 Mar 2018 2:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 27 17:05:20 2018

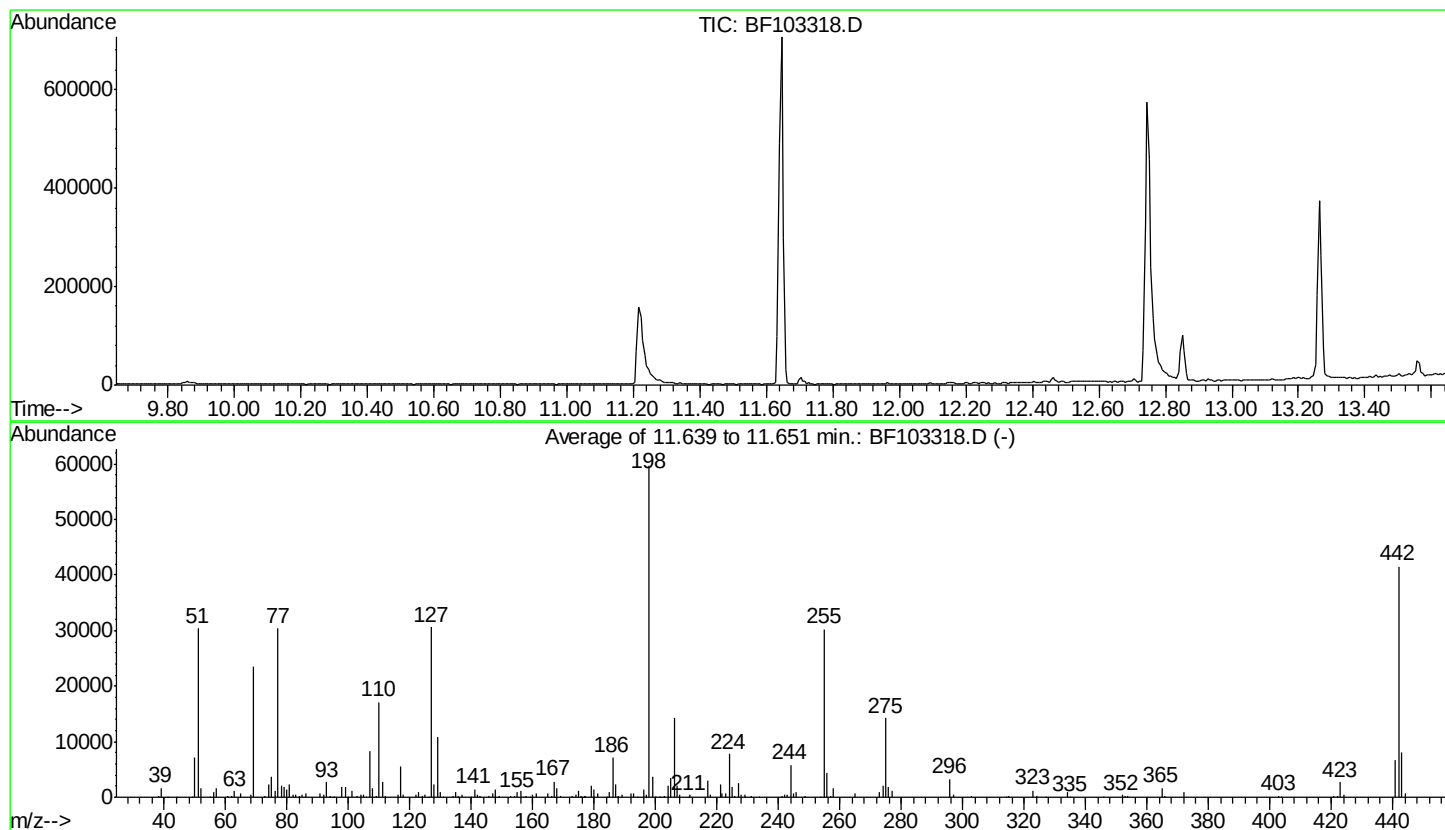

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.8	30350	PASS
68	69	0.00	2	1.8	419	PASS
69	198	0.00	100	39.6	23625	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	30585	PASS
197	198	0.00	2	0.9	552	PASS
198	198	100	100	100.0	59698	PASS
199	198	5	9	6.3	3782	PASS
275	198	10	60	23.8	14231	PASS
365	198	1	100	2.9	1729	PASS
441	443	0.01	100	83.2	6695	PASS
442	198	50	100	69.6	41552	PASS
443	442	15	24	19.4	8046	PASS