


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022820\
 Data File : BF119129.D
 Acq On : 28 Feb 2020 13:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 26 16:03:05 2020

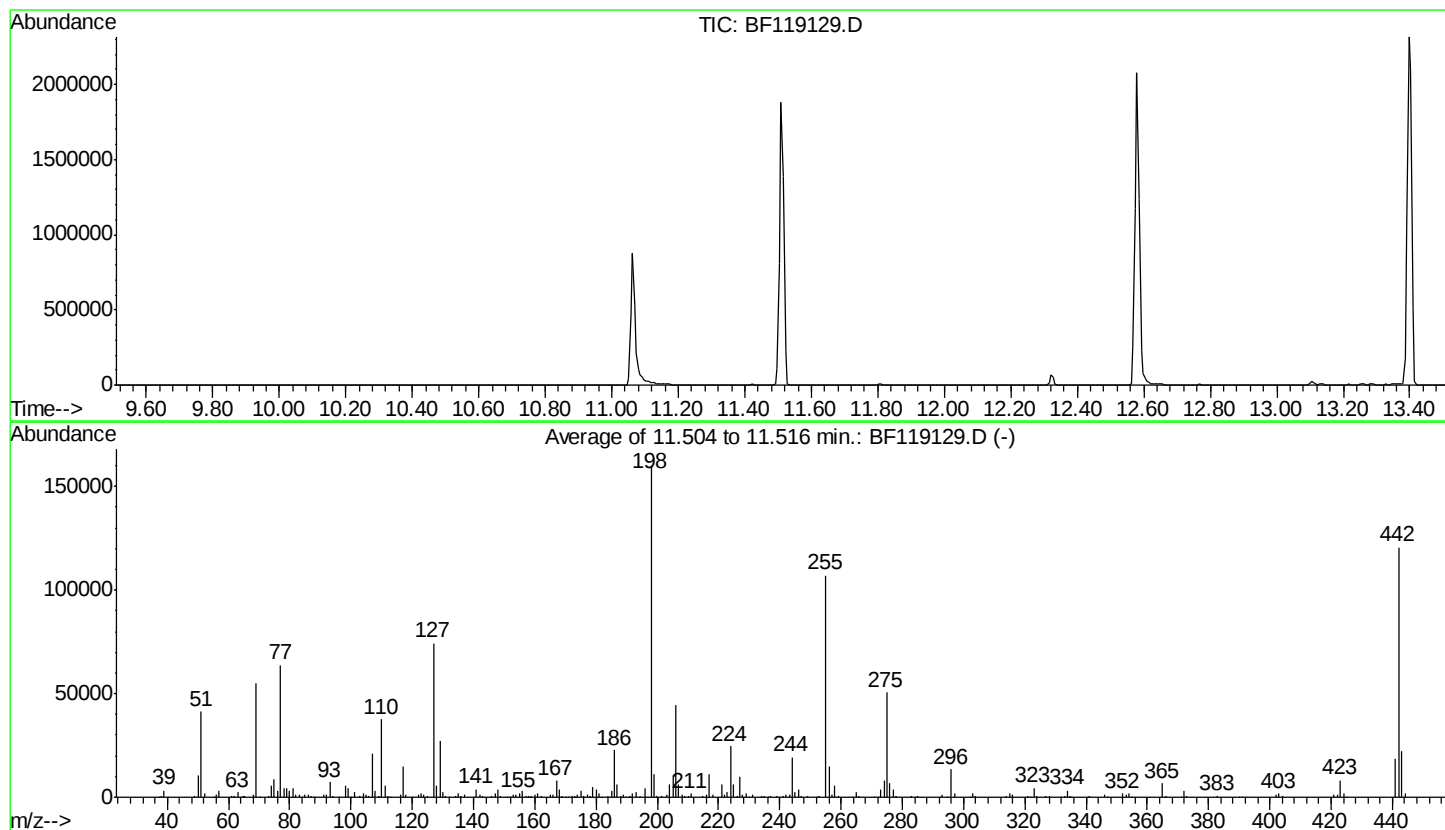

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	41346	PASS
68	69	0.00	2	2.0	1074	PASS
69	198	0.00	100	34.2	54728	PASS
70	69	0.00	2	0.2	123	PASS
127	198	10	80	46.4	74325	PASS
197	198	0.00	2	0.1	177	PASS
198	198	100	100	100.0	160058	PASS
199	198	5	9	6.8	10960	PASS
275	198	10	60	31.5	50426	PASS
365	198	1	100	4.2	6682	PASS
441	198	0.01	100	11.4	18322	PASS
442	198	50	100	75.5	120805	PASS
443	442	15	24	18.5	22357	PASS