
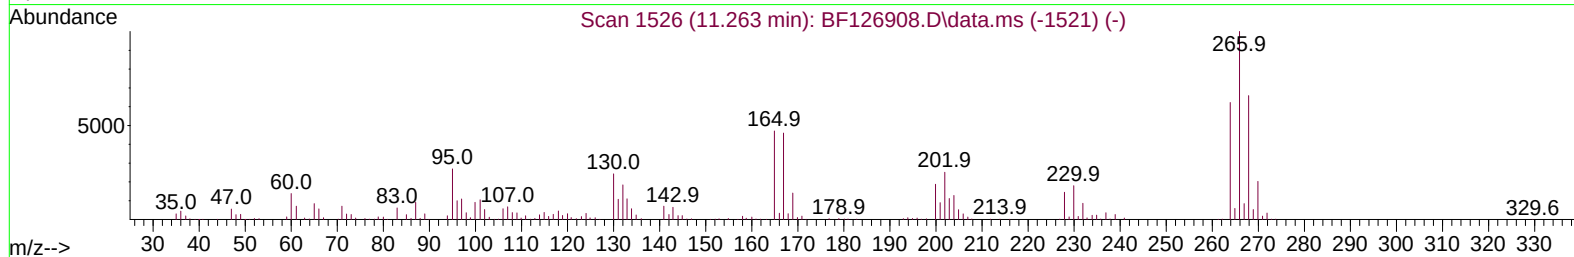
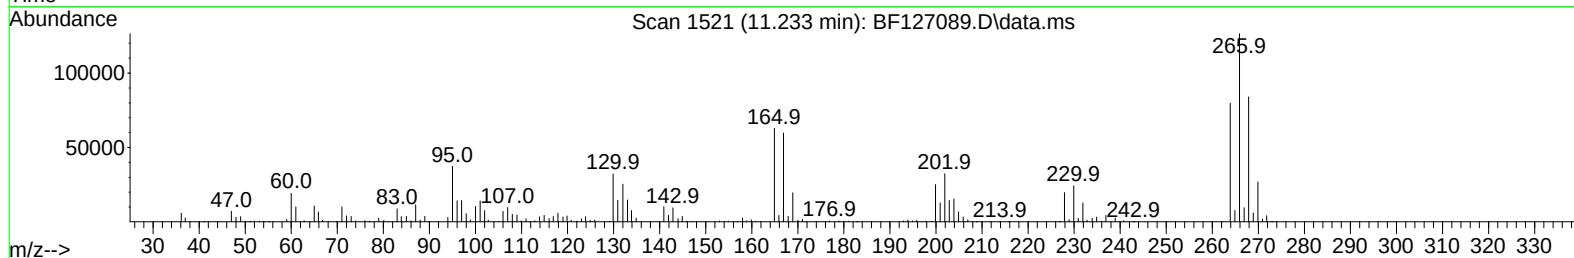


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022822\
Data File : BF127089.D
Acq On : 28 Feb 2022 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 16:49:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 24 02:10:57 2022
Response via : Initial Calibration

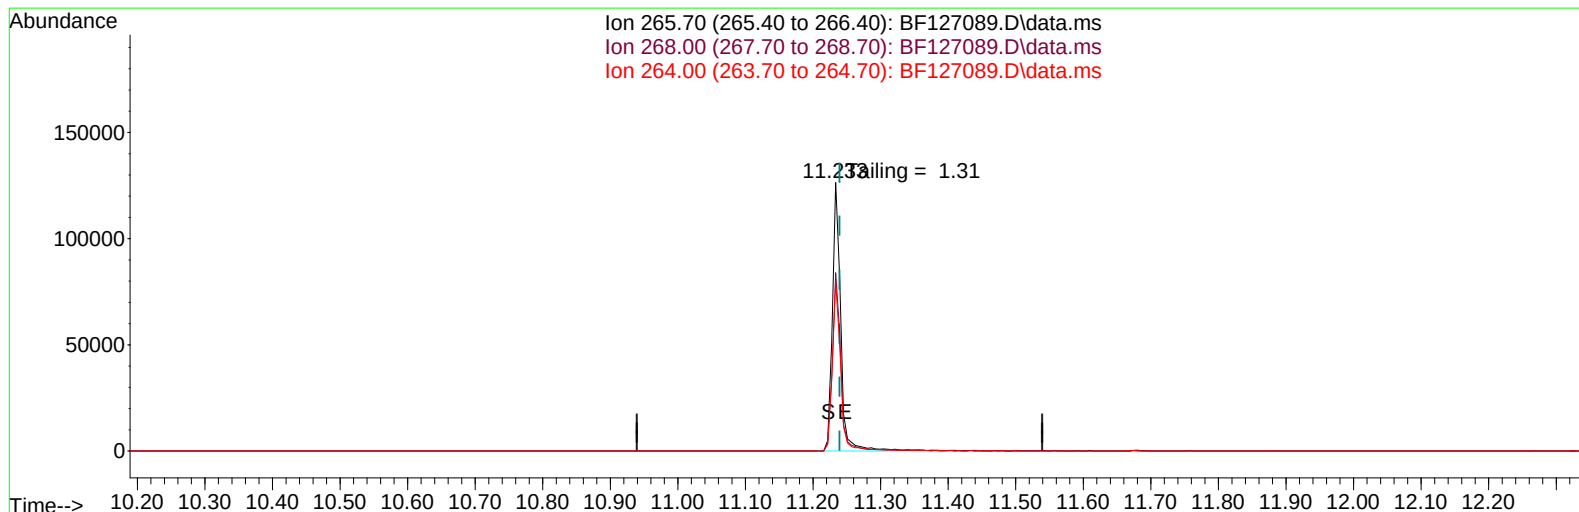

TIC: BF127089.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.006) 26248.55 ng

response 108234

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.41
264.00	63.00	63.14
0.00	0.00	0.00