
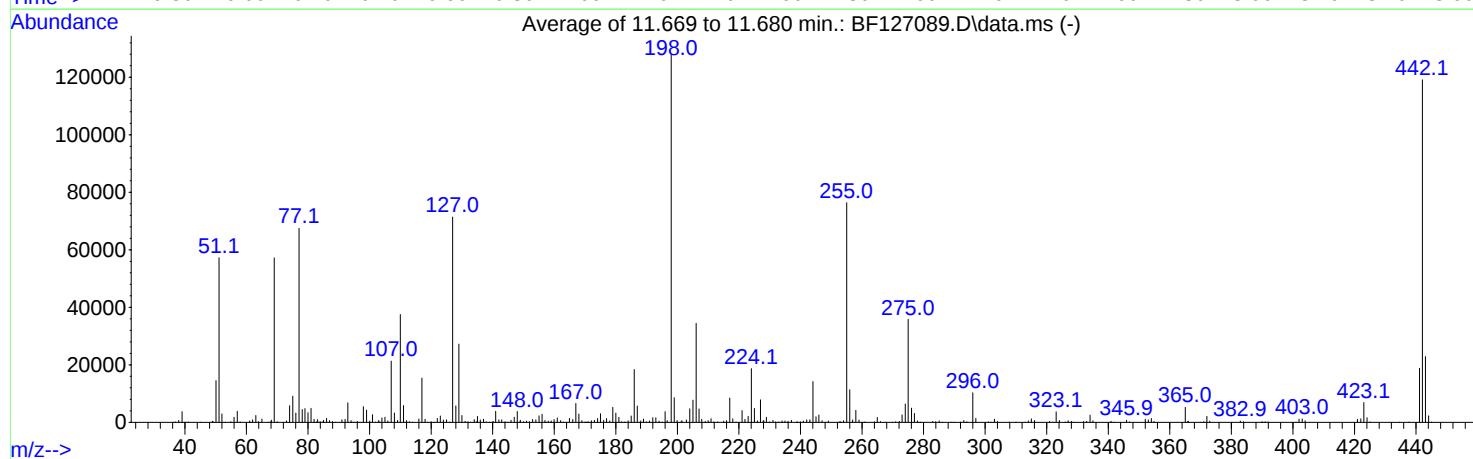


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022822\
 Data File : BF127089.D
 Acq On : 28 Feb 2022 09:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 24 02:10:57 2022

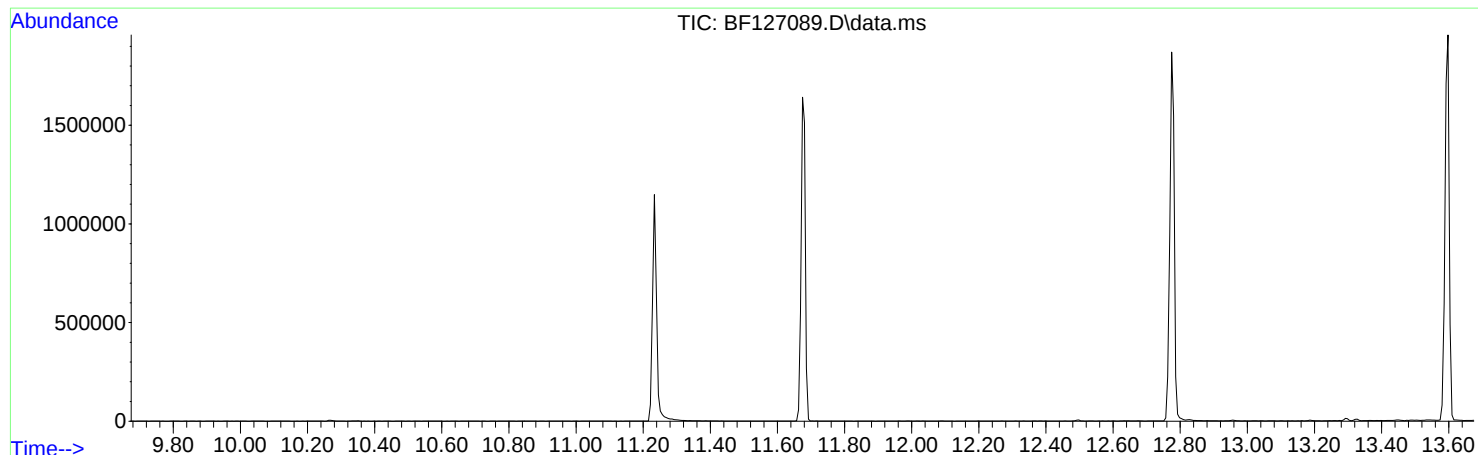




AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	57232	PASS
68	69	0.00	2	1.4	806	PASS
69	198	0.00	100	44.7	57213	PASS
70	69	0.00	2	0.4	232	PASS
127	198	10	80	55.8	71397	PASS
197	198	0.00	2	0.5	599	PASS
198	198	100	100	100.0	127923	PASS
199	198	5	9	6.7	8555	PASS
275	198	10	60	28.0	35808	PASS
365	198	1	100	4.1	5235	PASS
441	198	0.01	100	14.7	18786	PASS
442	198	50	100	93.1	119117	PASS
443	442	15	24	19.2	22869	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022822\
Data File : BF127089.D
Acq On : 28 Feb 2022 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 28 16:49:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 24 02:10:57 2022
Response via : Initial Calibration

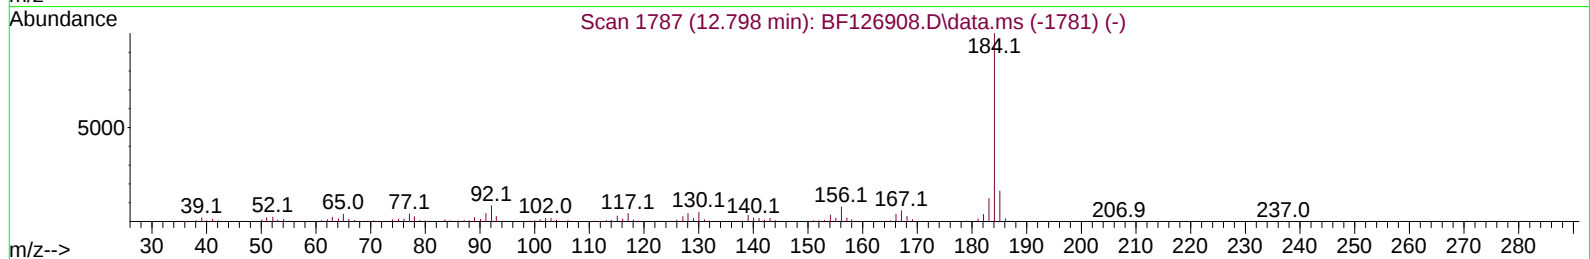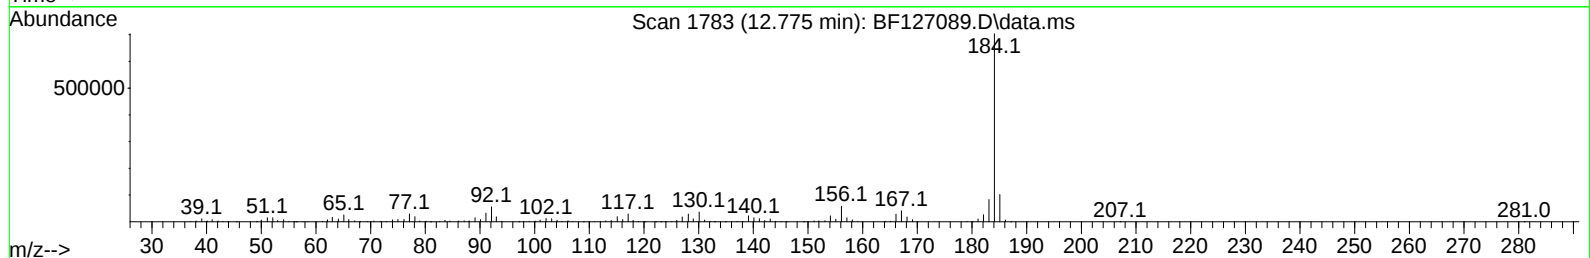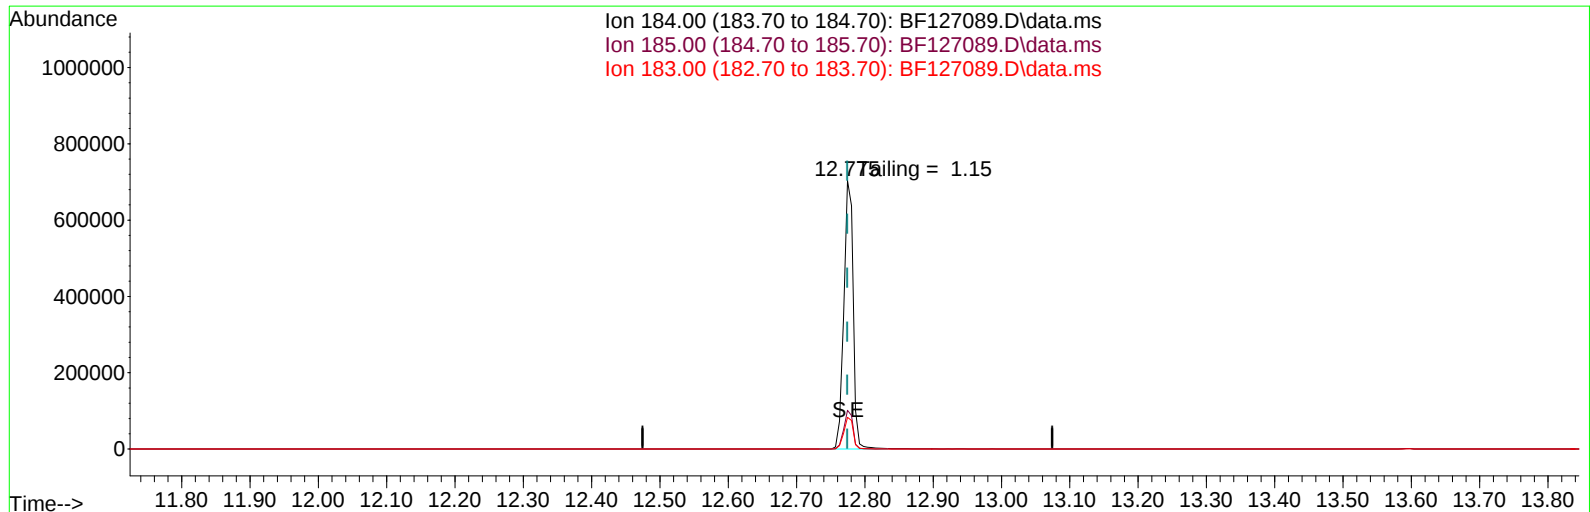

TIC: BF127089.D\data.ms

(77) Benzidine

12.775min (+ 0.000) 0.00 ng




response 671821

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.45
183.00	10.20	11.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022822\
 Data File : BF127089.D
 Acq On : 28 Feb 2022 09:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 28 16:49:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 24 02:10:57 2022
 Response via : Initial Calibration

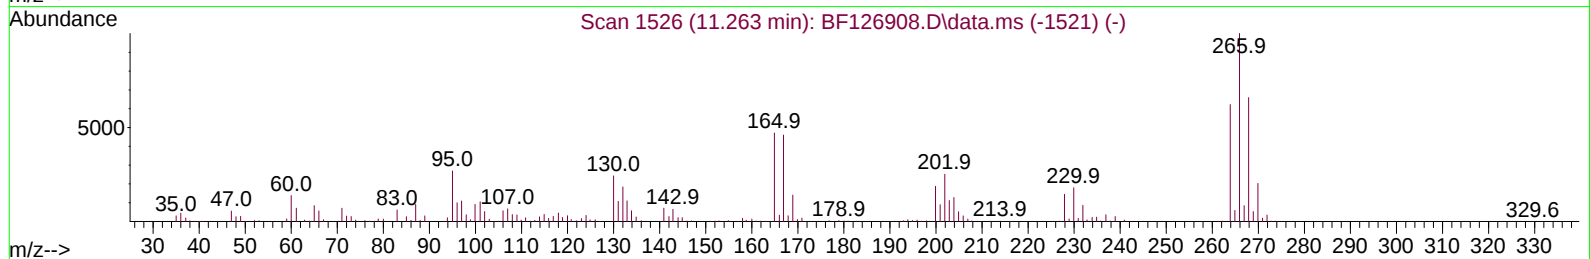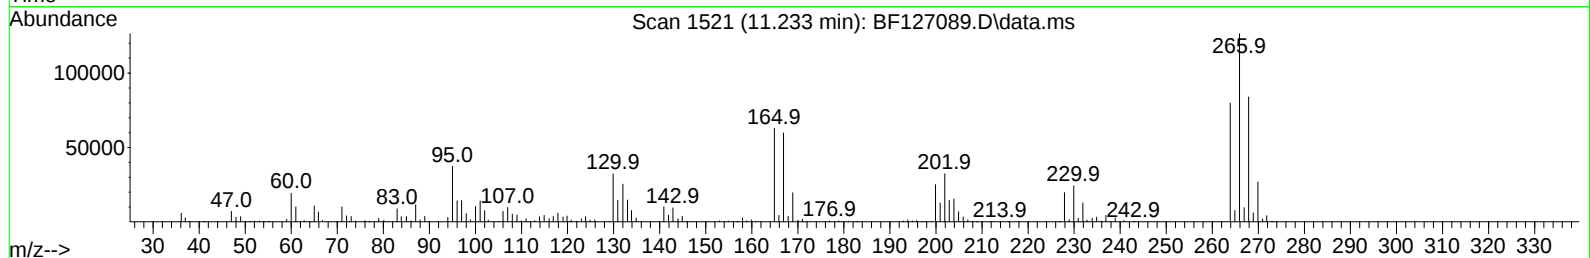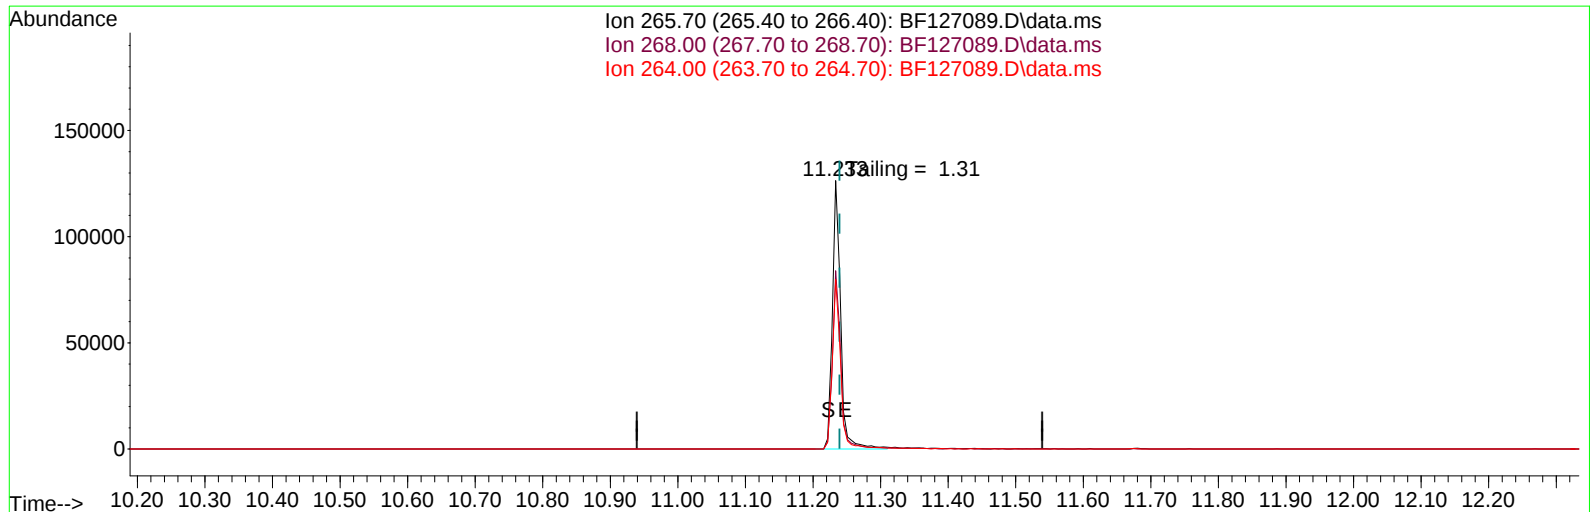

TIC: BF127089.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.006) 26248.55 ng

response 108234

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.41
264.00	63.00	63.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/28/2022	BNA_F	<u>BF127089.D</u>
Compound Name	Response	Retention Time
DDT	312265	23.59
DDD	2315	23.29
DDE	578	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2893	315158	0.92

Instrument :
BNA_F
ClientSampleId :
DFTPP