

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022824\
 Data File : BF137425.D
 Acq On : 28 Feb 2024 16:22
 Operator : CG\JU
 Sample : PB159325BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB159325BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.140	5	9	15	rVB	80566	101603	1.11%	0.182%
2	5.057	500	505	514	rBV	88309	142708	1.56%	0.256%
3	5.428	563	568	571	rBV	6896764	7494404	82.15%	13.455%
4	6.428	732	738	741	rBV	6249924	7807439	85.58%	14.018%
5	6.781	795	798	816	rBV	1858926	1611094	17.66%	2.893%
6	7.345	889	894	897	rBV	4707128	5092530	55.82%	9.143%
7	8.063	1011	1016	1034	rBV	2153387	2243806	24.60%	4.029%
8	9.145	1193	1200	1203	rBV	8196575	8690438	95.26%	15.603%
9	9.816	1309	1314	1318	rBV	2657603	2544395	27.89%	4.568%
10	10.616	1445	1450	1453	rBV	5202753	4690728	51.42%	8.422%
11	11.310	1564	1568	1588	rBV	2794504	2636869	28.90%	4.734%
12	12.922	1836	1842	1845	rBV	8688152	9122757	100.00%	16.379%
13	13.969	2016	2020	2033	rBV	2270266	2058458	22.56%	3.696%
14	15.457	2268	2273	2280	rBV	1162394	1460476	16.01%	2.622%




Sum of corrected areas: 55697705

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022824\
Data File : BF137425.D
Acq On : 28 Feb 2024 16:22
Operator : CG\JU
Sample : PB159325BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159325BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

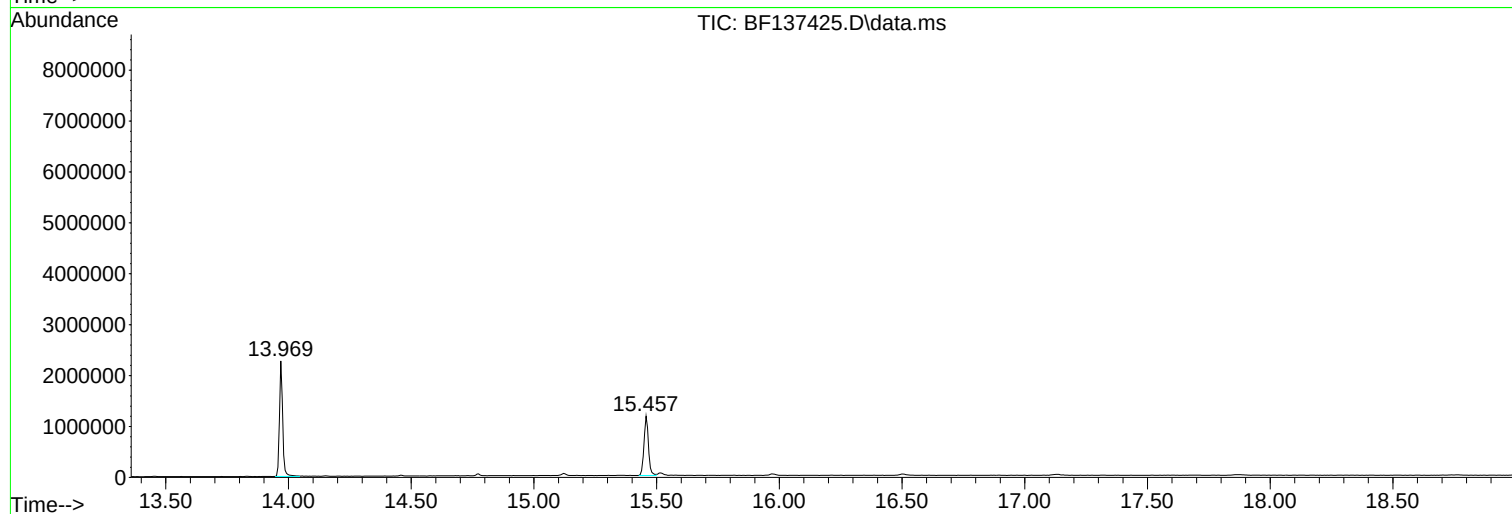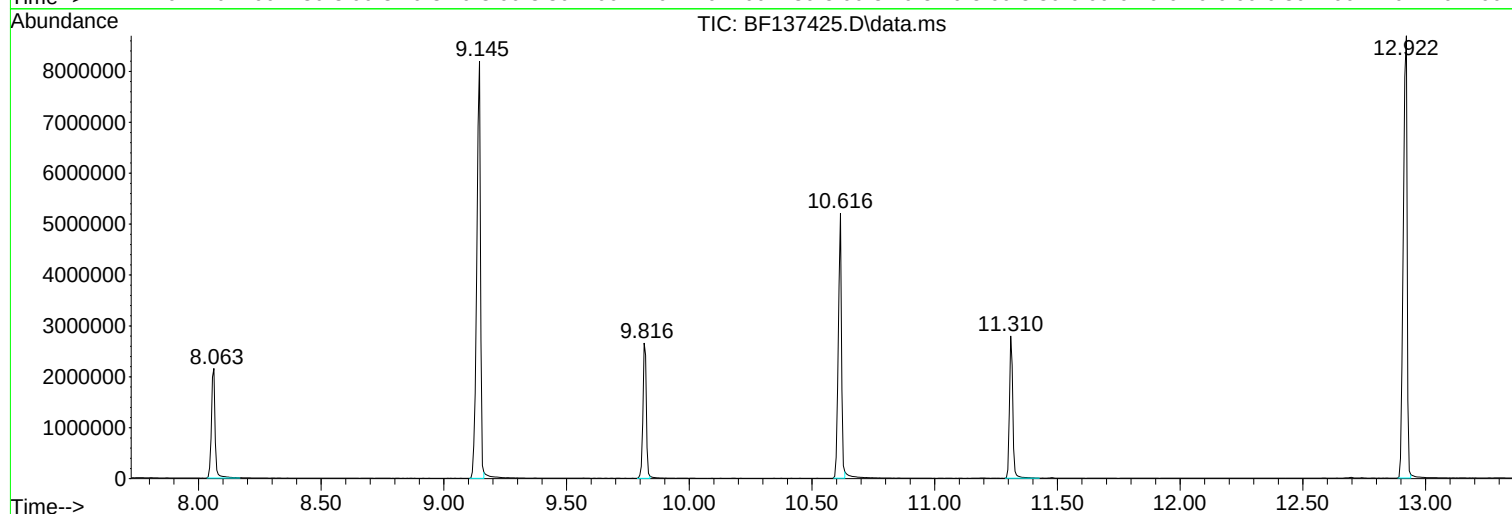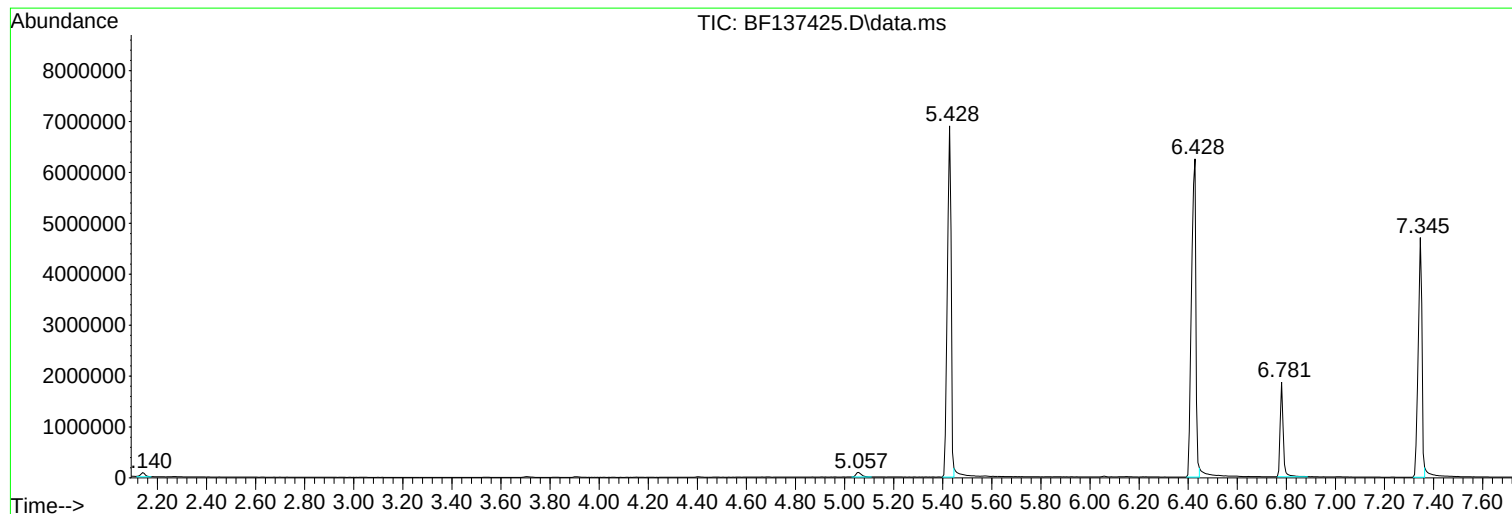

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022824\
Data File : BF137425.D
Acq On : 28 Feb 2024 16:22
Operator : CG\JU
Sample : PB159325BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159325BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022824\
Data File : BF137425.D
Acq On : 28 Feb 2024 16:22
Operator : CG\JU
Sample : PB159325BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159325BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------