

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022824\
 Data File : BF137436.D
 Acq On : 28 Feb 2024 21:48
 Operator : CG\JU
 Sample : P1538-12RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20241105-AMENDED-COMPOSITE-35N-N-4-04RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	488	501	504	rBV	6449299	15834809	100.00%	49.179%
2	5.404	561	564	578	rBV	483905	519553	3.28%	1.614%
3	6.410	732	735	748	rBV2	971697	1193902	7.54%	3.708%
4	6.781	794	798	806	rBV	682999	621387	3.92%	1.930%
5	7.339	890	893	908	rBV	1461629	1336228	8.44%	4.150%
6	7.492	916	919	925	rBV	368922	365777	2.31%	1.136%
7	8.063	1012	1016	1024	rBV	954461	901681	5.69%	2.800%
8	9.139	1195	1199	1202	rBV	3323990	2544717	16.07%	7.903%
9	9.816	1311	1314	1324	rVB	1352108	1188303	7.50%	3.691%
10	10.610	1446	1449	1456	rBV	248876	243555	1.54%	0.756%
11	10.733	1466	1470	1475	rBV	376490	351021	2.22%	1.090%
12	11.180	1542	1546	1549	rBV	207152	194681	1.23%	0.605%
13	11.310	1565	1568	1577	rBV	1528982	1349160	8.52%	4.190%
14	12.910	1836	1840	1844	rBV	3556822	3221471	20.34%	10.005%
15	13.821	1992	1995	2003	rBV2	254565	296322	1.87%	0.920%
16	13.968	2016	2020	2032	rVB	1185003	1154655	7.29%	3.586%
17	15.457	2268	2273	2280	rBV	669983	881117	5.56%	2.737%




Sum of corrected areas: 32198339

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022824\
Data File : BF137436.D
Acq On : 28 Feb 2024 21:48
Operator : CG\JU
Sample : P1538-12RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20241105-AMENDED-COMPOSITE-35N-N-4-04RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

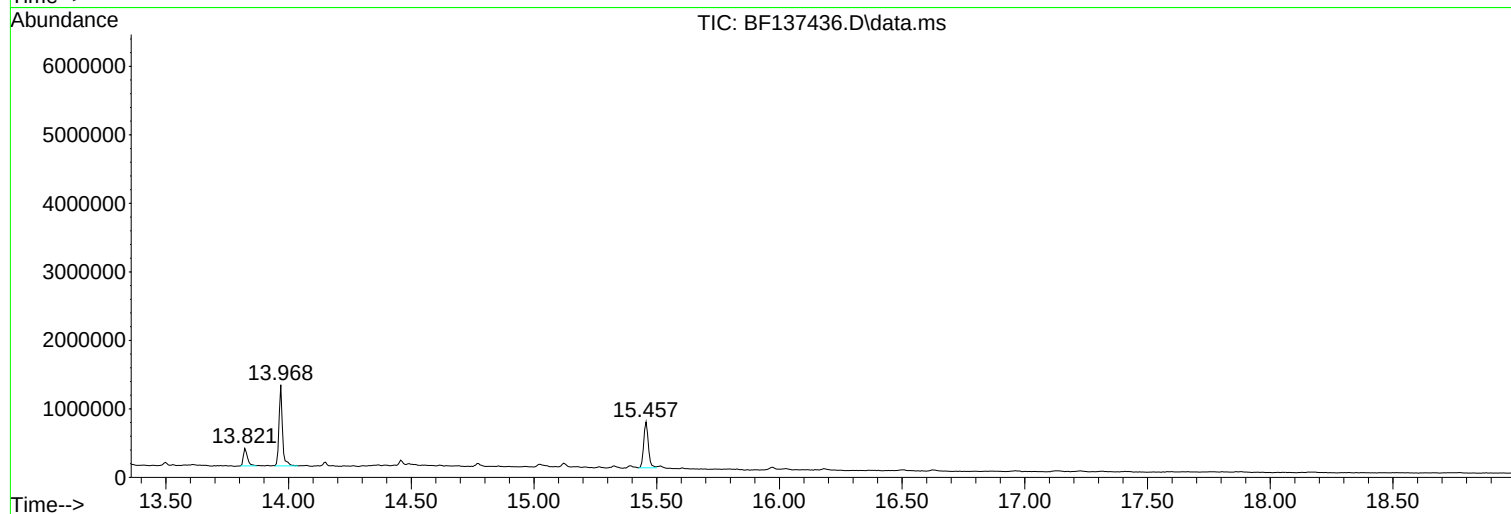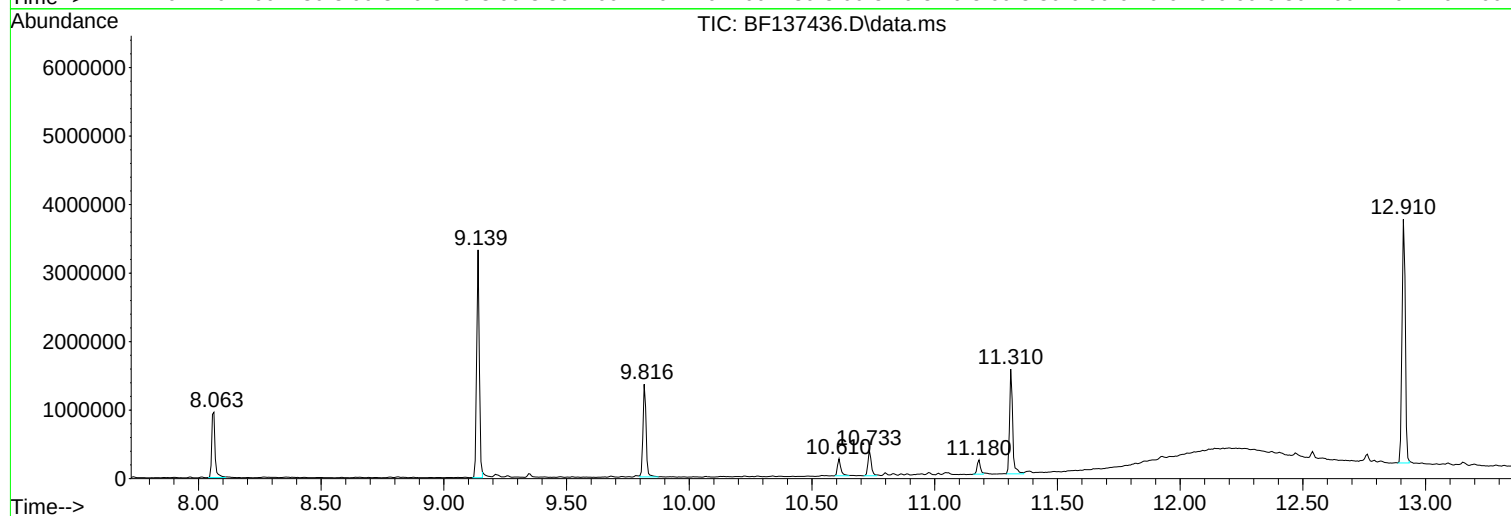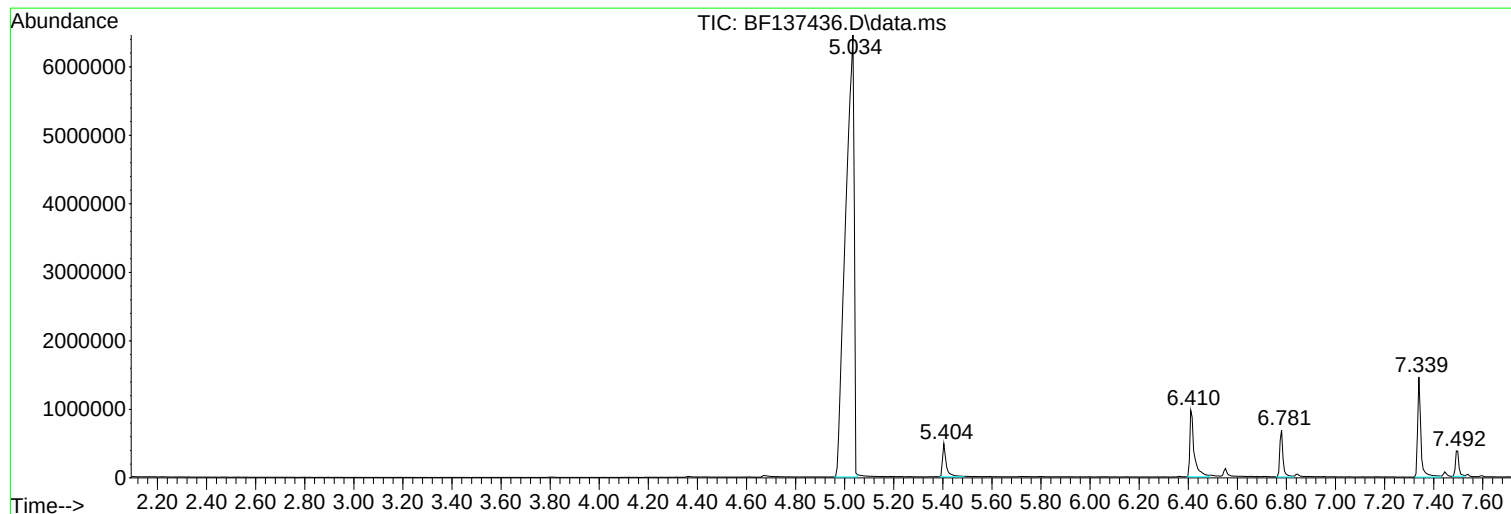

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022824\
Data File : BF137436.D
Acq On : 28 Feb 2024 21:48
Operator : CG\JU
Sample : P1538-12RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20241105-AMENDED-COMPOSITE-35N-N-4-04RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022824\
Data File : BF137436.D
Acq On : 28 Feb 2024 21:48
Operator : CG\JU
Sample : P1538-12RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20241105-AMENDED-COMPOSITE-35N-N-4-04RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------