
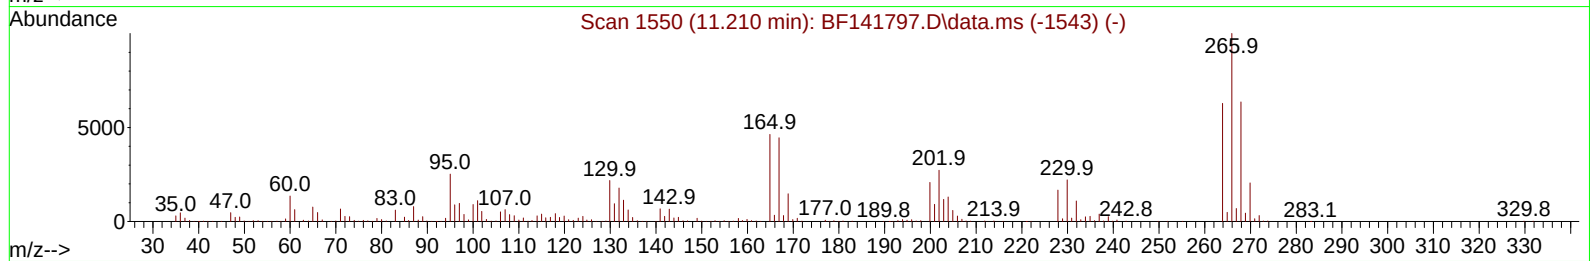
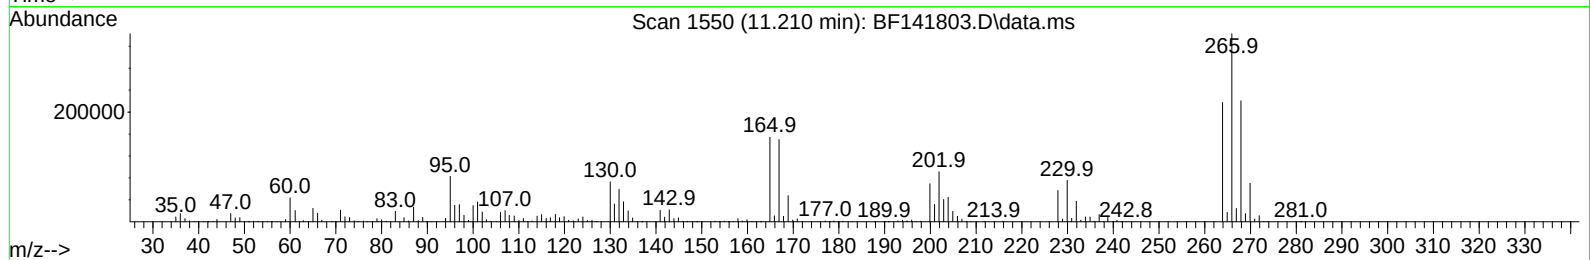


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022825\
Data File : BF141803.D
Acq On : 28 Feb 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 11:14:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

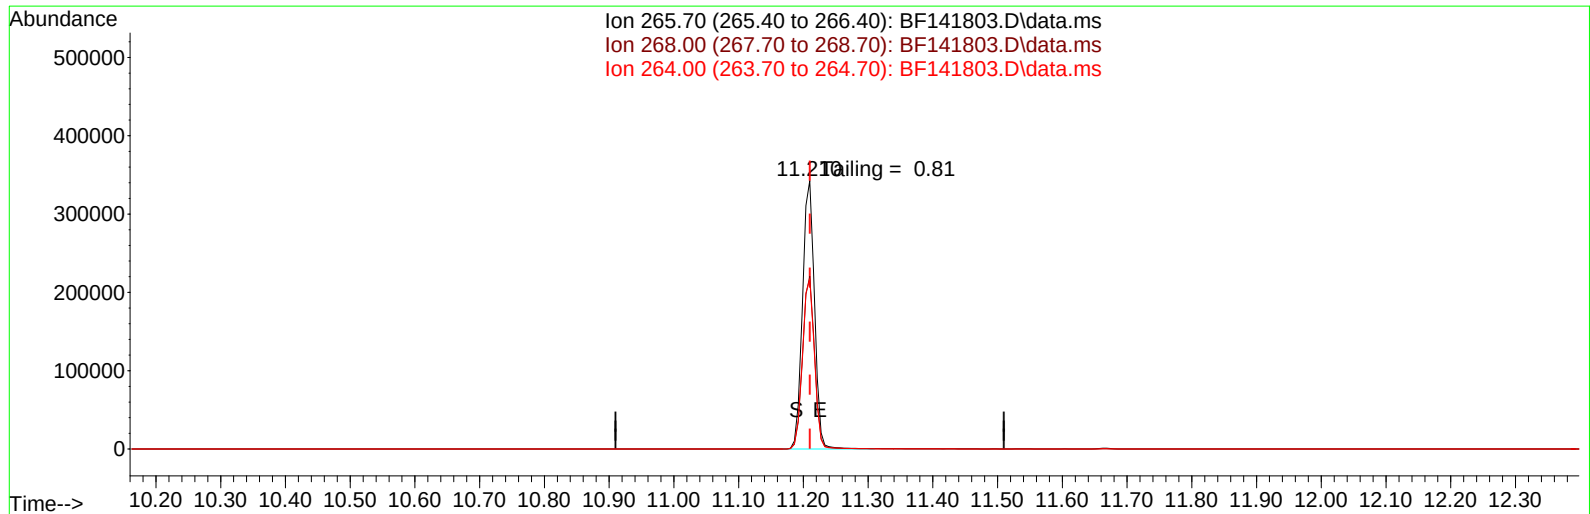

TIC: BF141803.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 17699.40 ng

response 444866

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.33
264.00	62.80	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022825\
Data File : BF141803.D
Acq On : 28 Feb 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 11:14:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

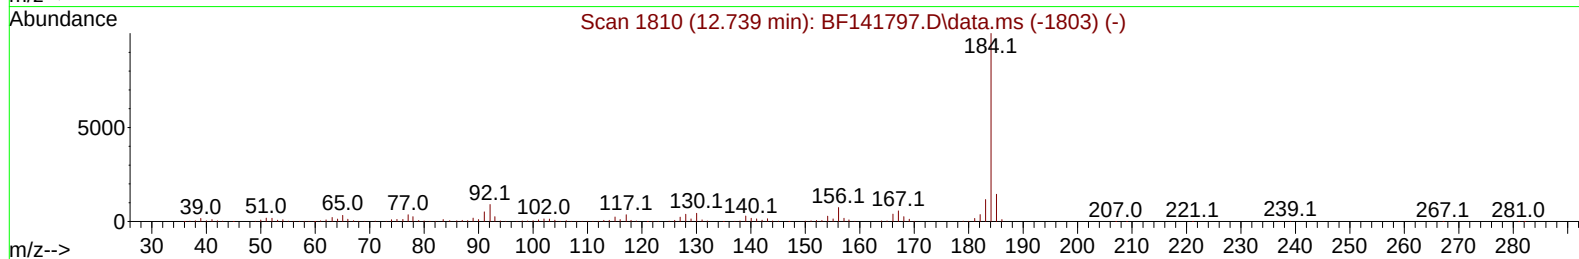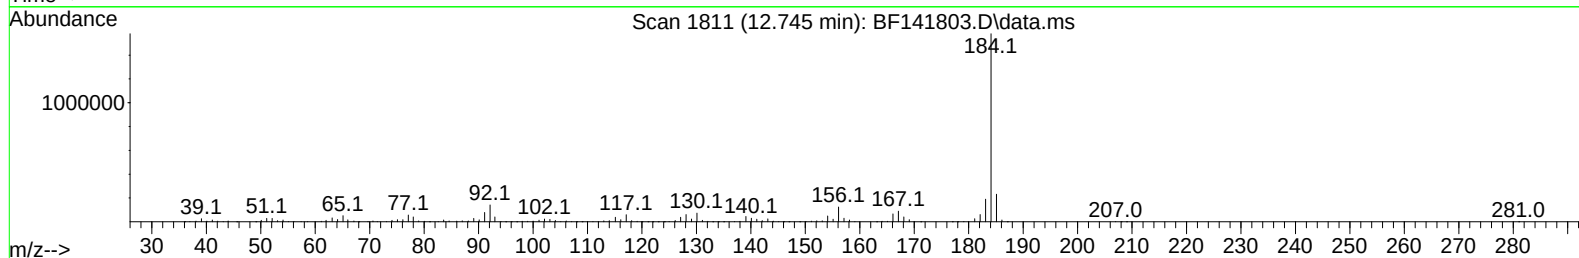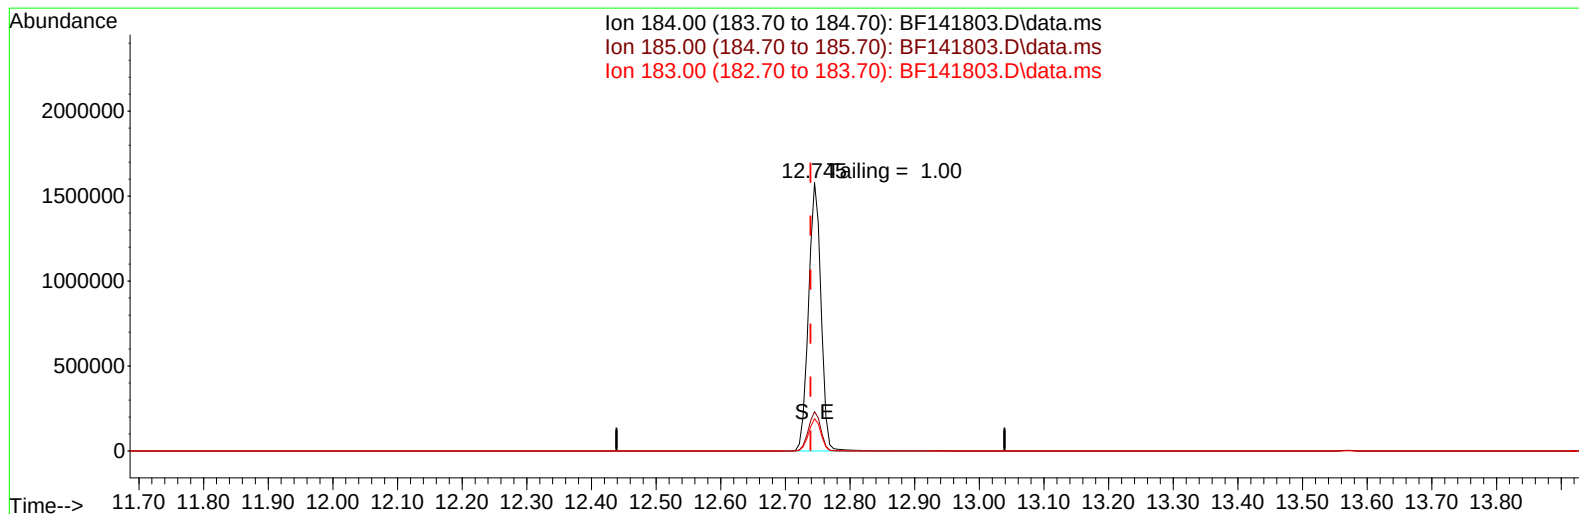

TIC: BF141803.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 81741.12 ng

response 2125556

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.68
183.00	11.70	12.05
0.00	0.00	0.00