


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022920\
 Data File : BF119154.D
 Acq On : 29 Feb 2020 12:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 26 16:03:05 2020

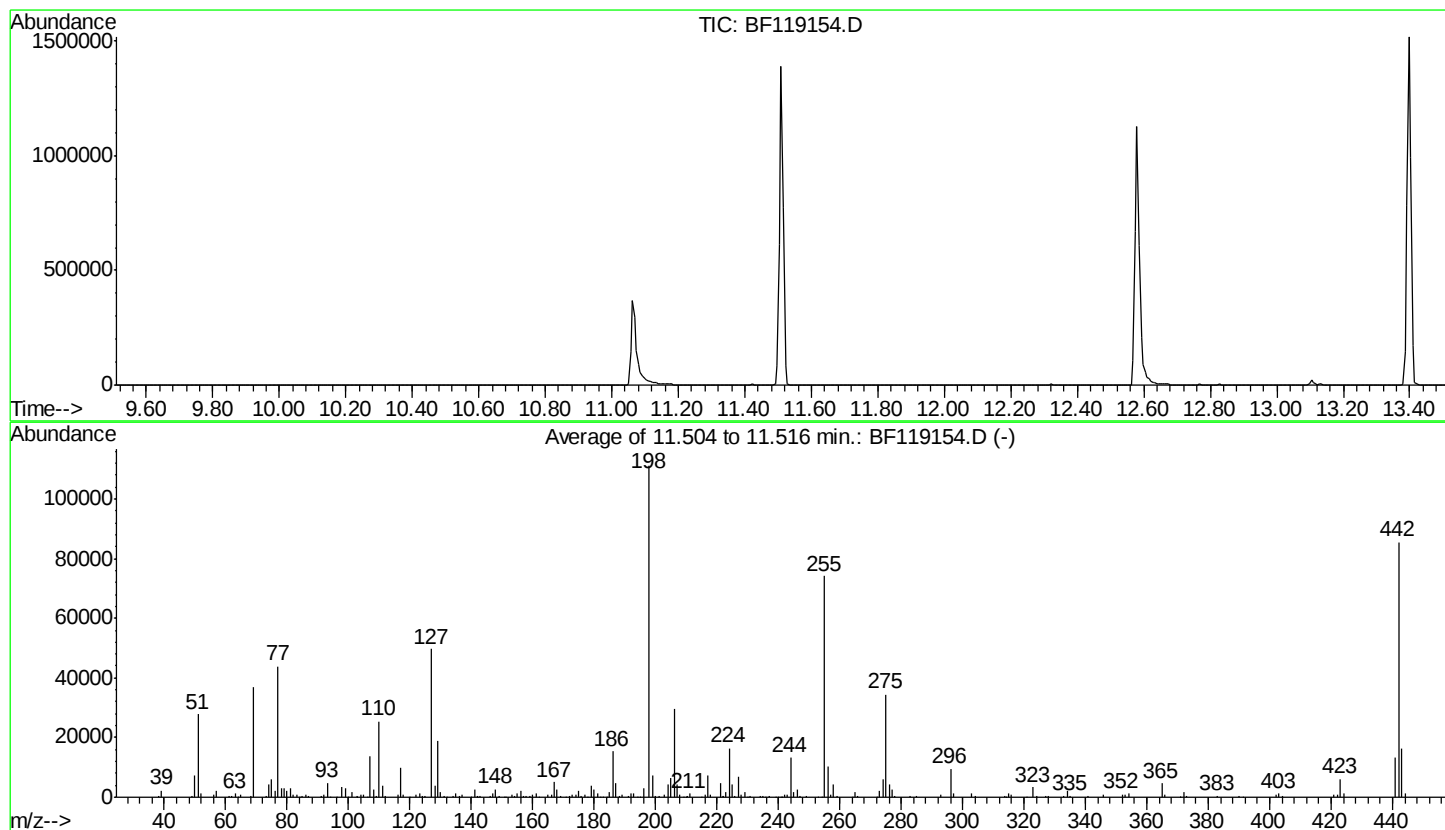

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	27854	PASS
68	69	0.00	2	1.7	637	PASS
69	198	0.00	100	33.2	36893	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.6	49602	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111162	PASS
199	198	5	9	6.8	7515	PASS
275	198	10	60	31.0	34512	PASS
365	198	1	100	4.2	4637	PASS
441	198	0.01	100	12.1	13427	PASS
442	198	50	100	76.9	85445	PASS
443	442	15	24	18.9	16171	PASS