


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030116\
 Data File : BF085096.D
 Acq On : 1 Mar 2016 17:39
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 02 13:25:39 2016

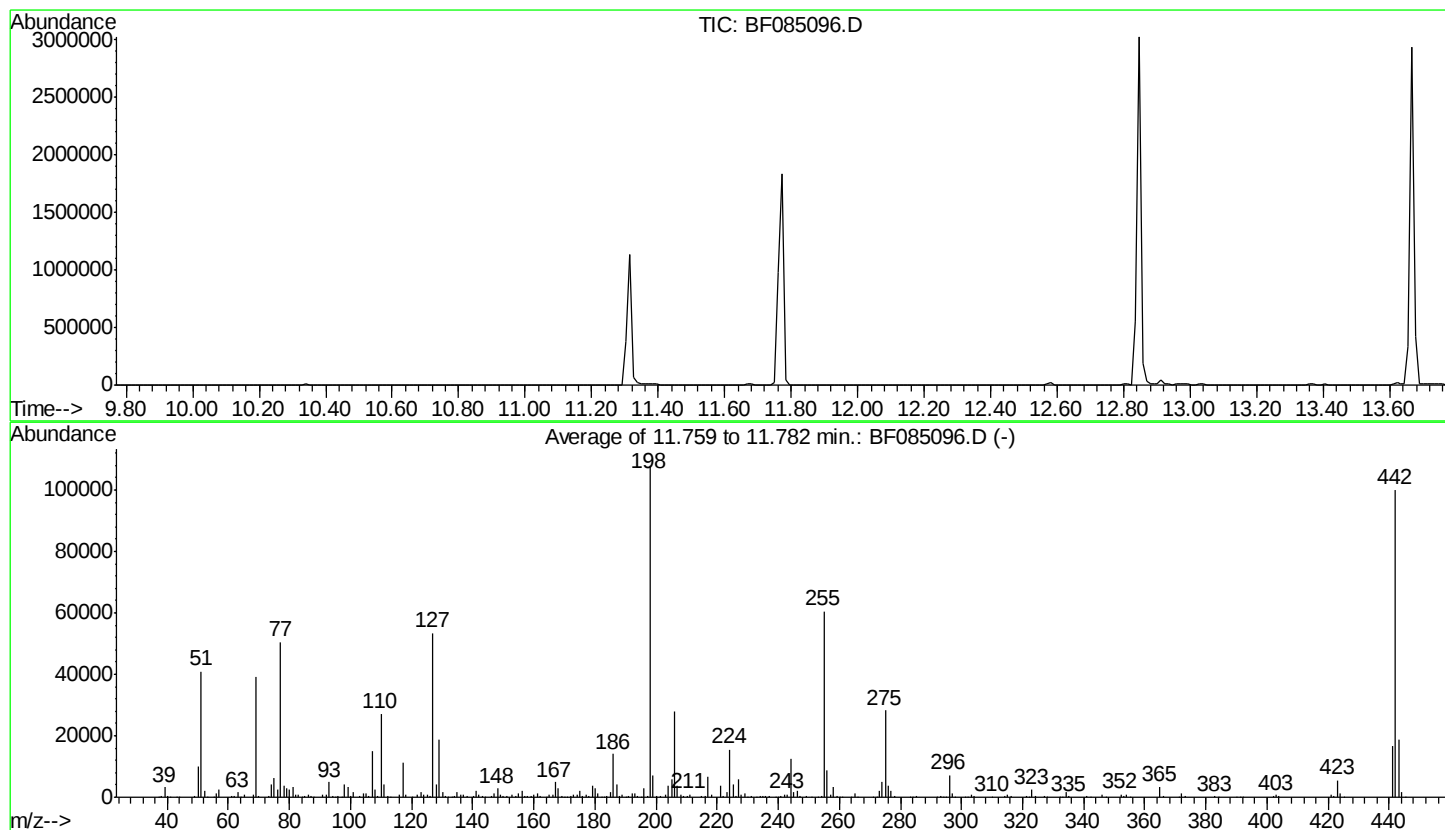

AutoFind: Scans 890, 891, 892; Background Corrected with Scan 886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	40957	PASS
68	69	0.00	2	2.0	784	PASS
69	198	0.00	100	36.5	39356	PASS
70	69	0.00	2	0.8	305	PASS
127	198	10	80	49.5	53378	PASS
197	198	0.00	2	0.6	634	PASS
198	198	100	100	100.0	107886	PASS
199	198	5	9	6.8	7291	PASS
275	198	10	60	26.1	28198	PASS
365	198	1	100	3.3	3552	PASS
441	442	0.01	24	16.4	16466	PASS
442	198	50	100	92.8	100114	PASS
443	442	15	24	18.8	18855	PASS