
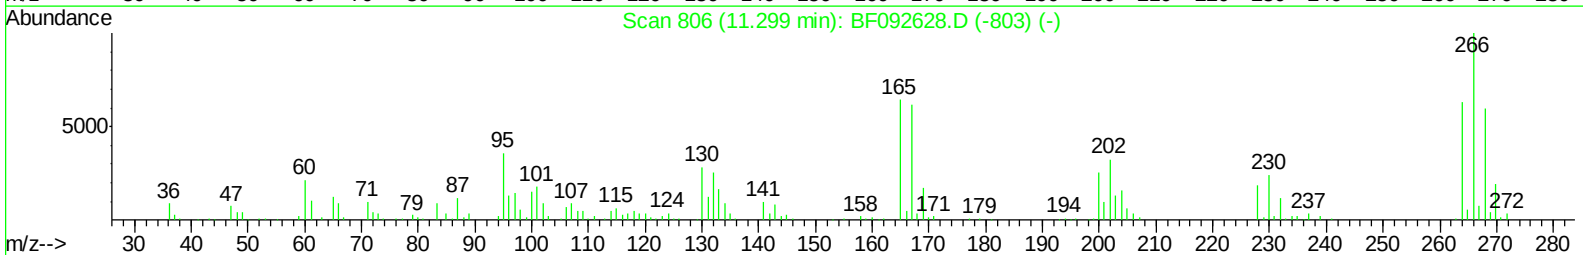
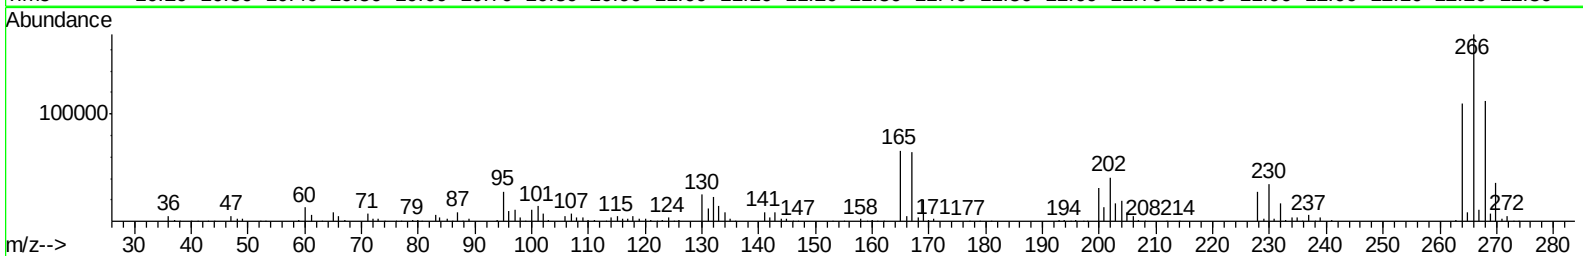


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030117\
Data File : BF093287.D
Acq On : 1 Mar 2017 13:58
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 02 03:09:23 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

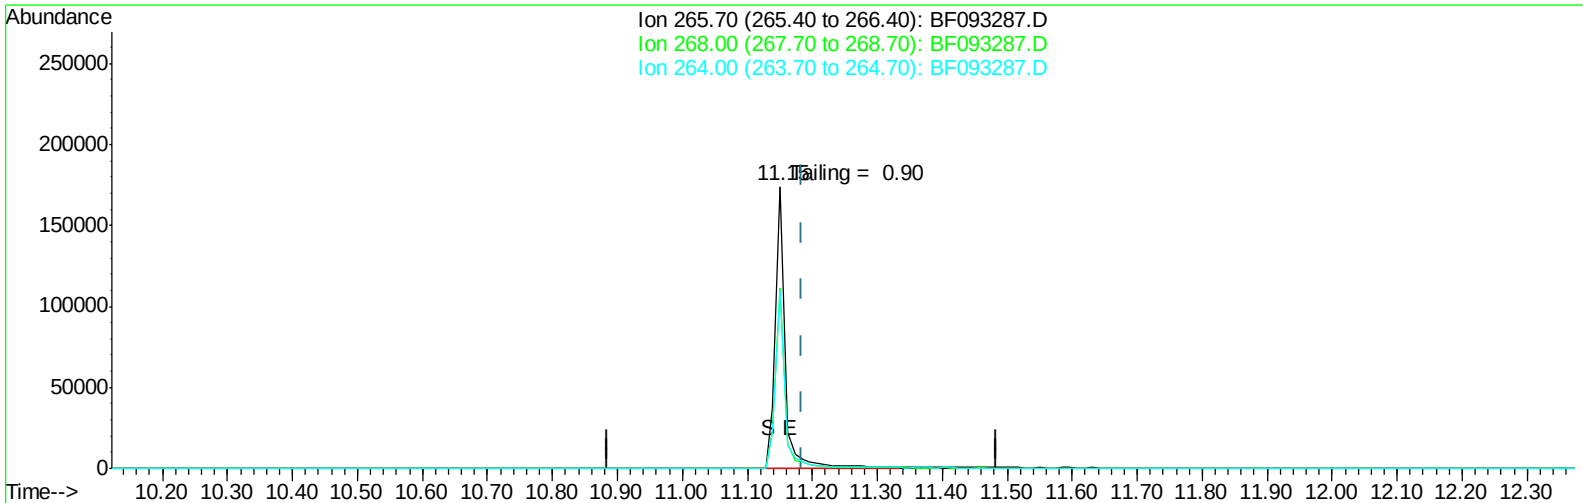

TIC: BF093287.D

(69) Pentachlorophenol (C)




11.151min (-0.034) 61354.61ng

response 186841

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.18
264.00	62.90	63.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030117\
 Data File : BF093287.D
 Acq On : 1 Mar 2017 13:58
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 02 03:09:23 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 17:31:55 2017
 Response via : Initial Calibration

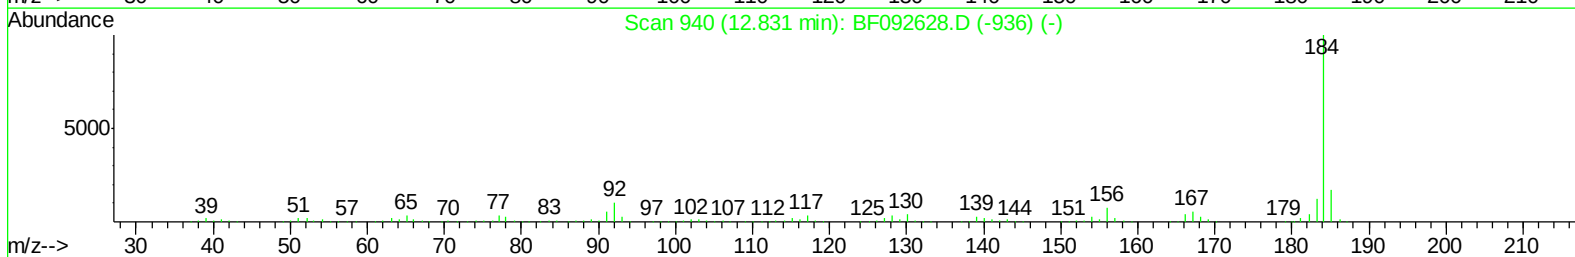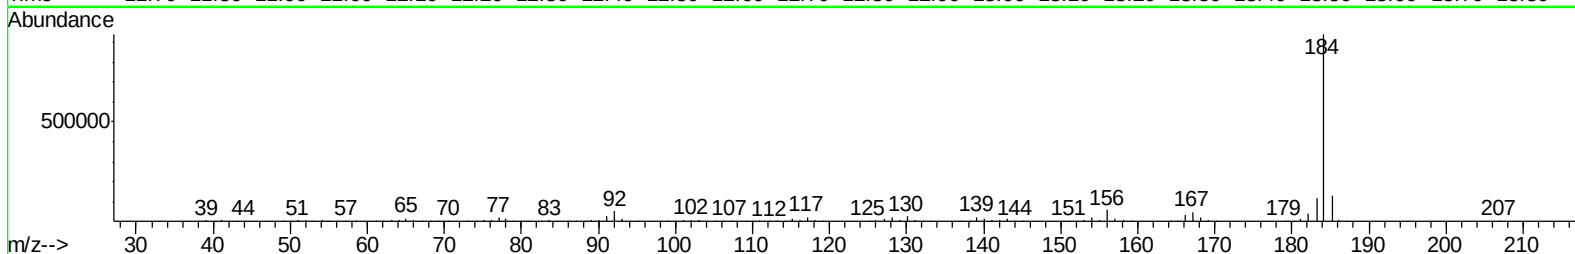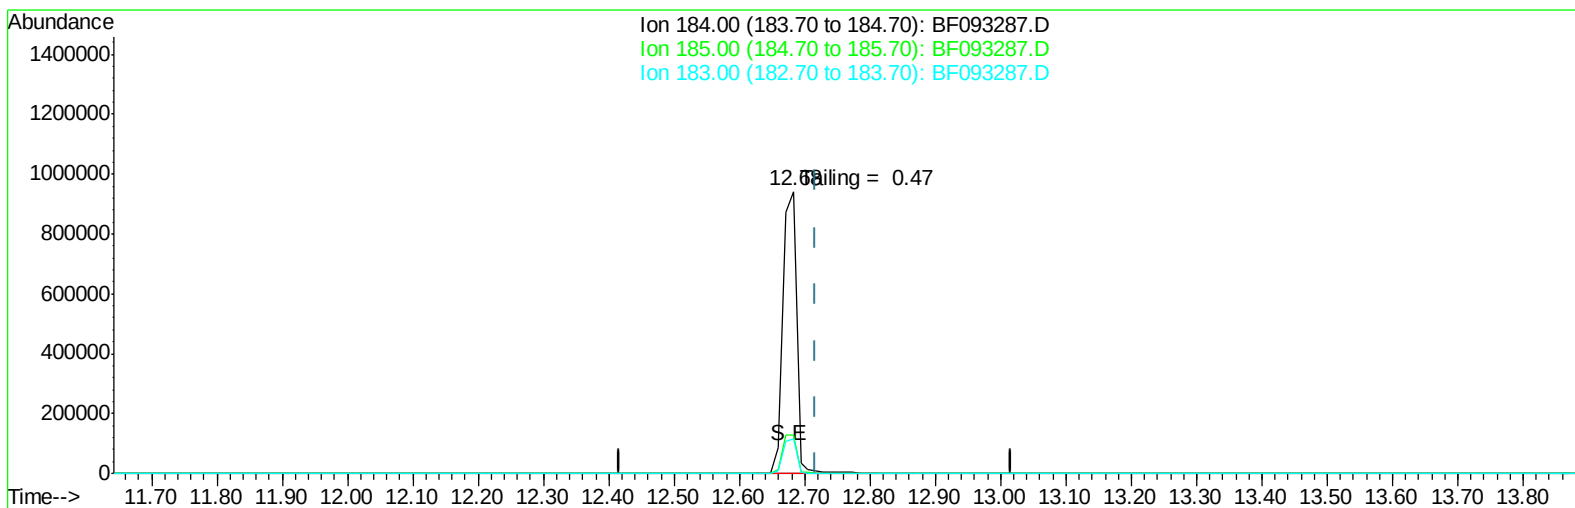

TIC: BF093287.D

(76) Benzidine

12.682min (-0.034) 0.00ng

response 1364295

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	13.86
183.00	11.50	12.16
0.00	0.00	0.00