


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030117\
 Data File : BF093287.D
 Acq On : 1 Mar 2017 13:58
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

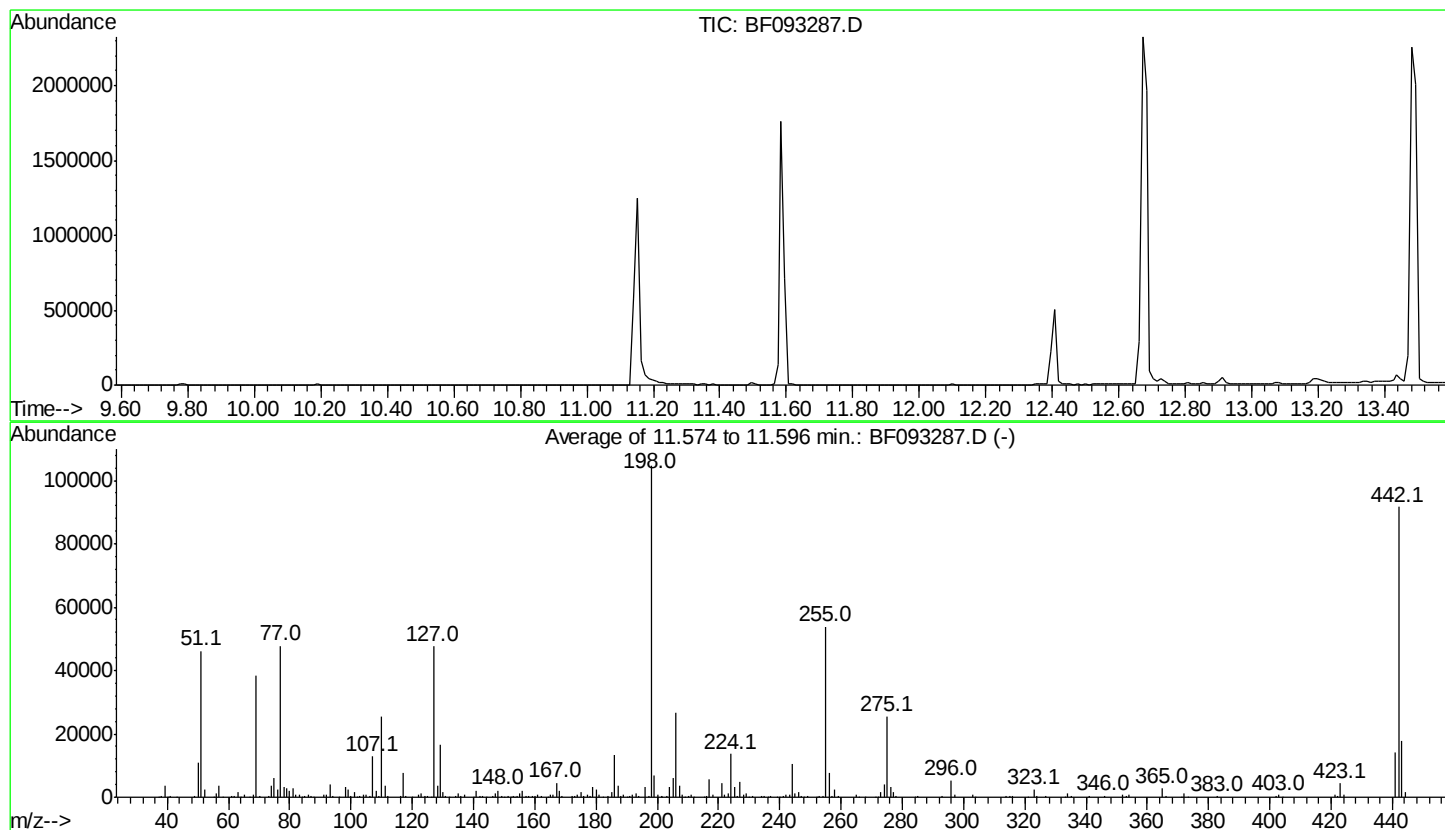

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	46287	PASS
68	69	0.00	2	1.7	640	PASS
69	198	0.00	100	36.7	38399	PASS
70	69	0.00	2	0.6	224	PASS
127	198	10	80	45.4	47533	PASS
197	198	0.00	2	0.2	237	PASS
198	198	100	100	100.0	104687	PASS
199	198	5	9	6.5	6841	PASS
275	198	10	60	24.2	25311	PASS
365	198	1	100	2.5	2646	PASS
441	442	0.01	24	15.7	14351	PASS
442	198	50	100	87.5	91621	PASS
443	442	15	24	19.6	17952	PASS