

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030118\
 Data File : BF103326.D
 Acq On : 1 Mar 2018 10:36
 Operator : SJ/JU
 Sample : PB106938BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB106938BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.199	11	19	24	rBV	32823	46867	1.11%	0.132%
2	5.122	513	516	529	rBV	97687	138622	3.29%	0.390%
3	5.504	577	581	595	rBV	3662018	4200727	99.72%	11.829%
4	6.510	747	752	768	rBV	3374746	4117376	97.74%	11.595%
5	6.645	771	775	779	rBV	3866952	3950018	93.77%	11.123%
6	6.869	810	813	828	rVB	1026657	956077	22.70%	2.692%
7	7.028	836	840	844	rBV	3238296	3082939	73.19%	8.682%
8	7.440	905	910	913	rBV	2649265	2746332	65.20%	7.734%
9	8.157	1027	1032	1045	rBV	1240337	1272950	30.22%	3.585%
10	9.228	1209	1214	1228	rBV	3739861	4212429	100.00%	11.862%
11	9.910	1326	1330	1340	rBV	1286572	1352301	32.10%	3.808%
12	10.710	1461	1466	1479	rBV	2242891	2491292	59.14%	7.015%
13	11.404	1580	1584	1596	rBV	1420613	1316589	31.25%	3.708%
14	11.710	1632	1636	1640	rBV7	21526	43712	1.04%	0.123%
15	11.822	1648	1655	1657	rBV8	19634	43826	1.04%	0.123%
16	12.163	1711	1713	1722	rVB4	39587	58429	1.39%	0.165%
17	12.992	1849	1854	1857	rBV	3351404	3679092	87.34%	10.360%
18	14.057	2030	2035	2043	rBV	920507	1063741	25.25%	2.995%
19	15.557	2285	2290	2301	rVB	465264	737982	17.52%	2.078%


Sum of corrected areas: 35511301

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030118\
Data File : BF103326.D
Acq On : 1 Mar 2018 10:36
Operator : SJ/JU
Sample : PB106938BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB106938BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

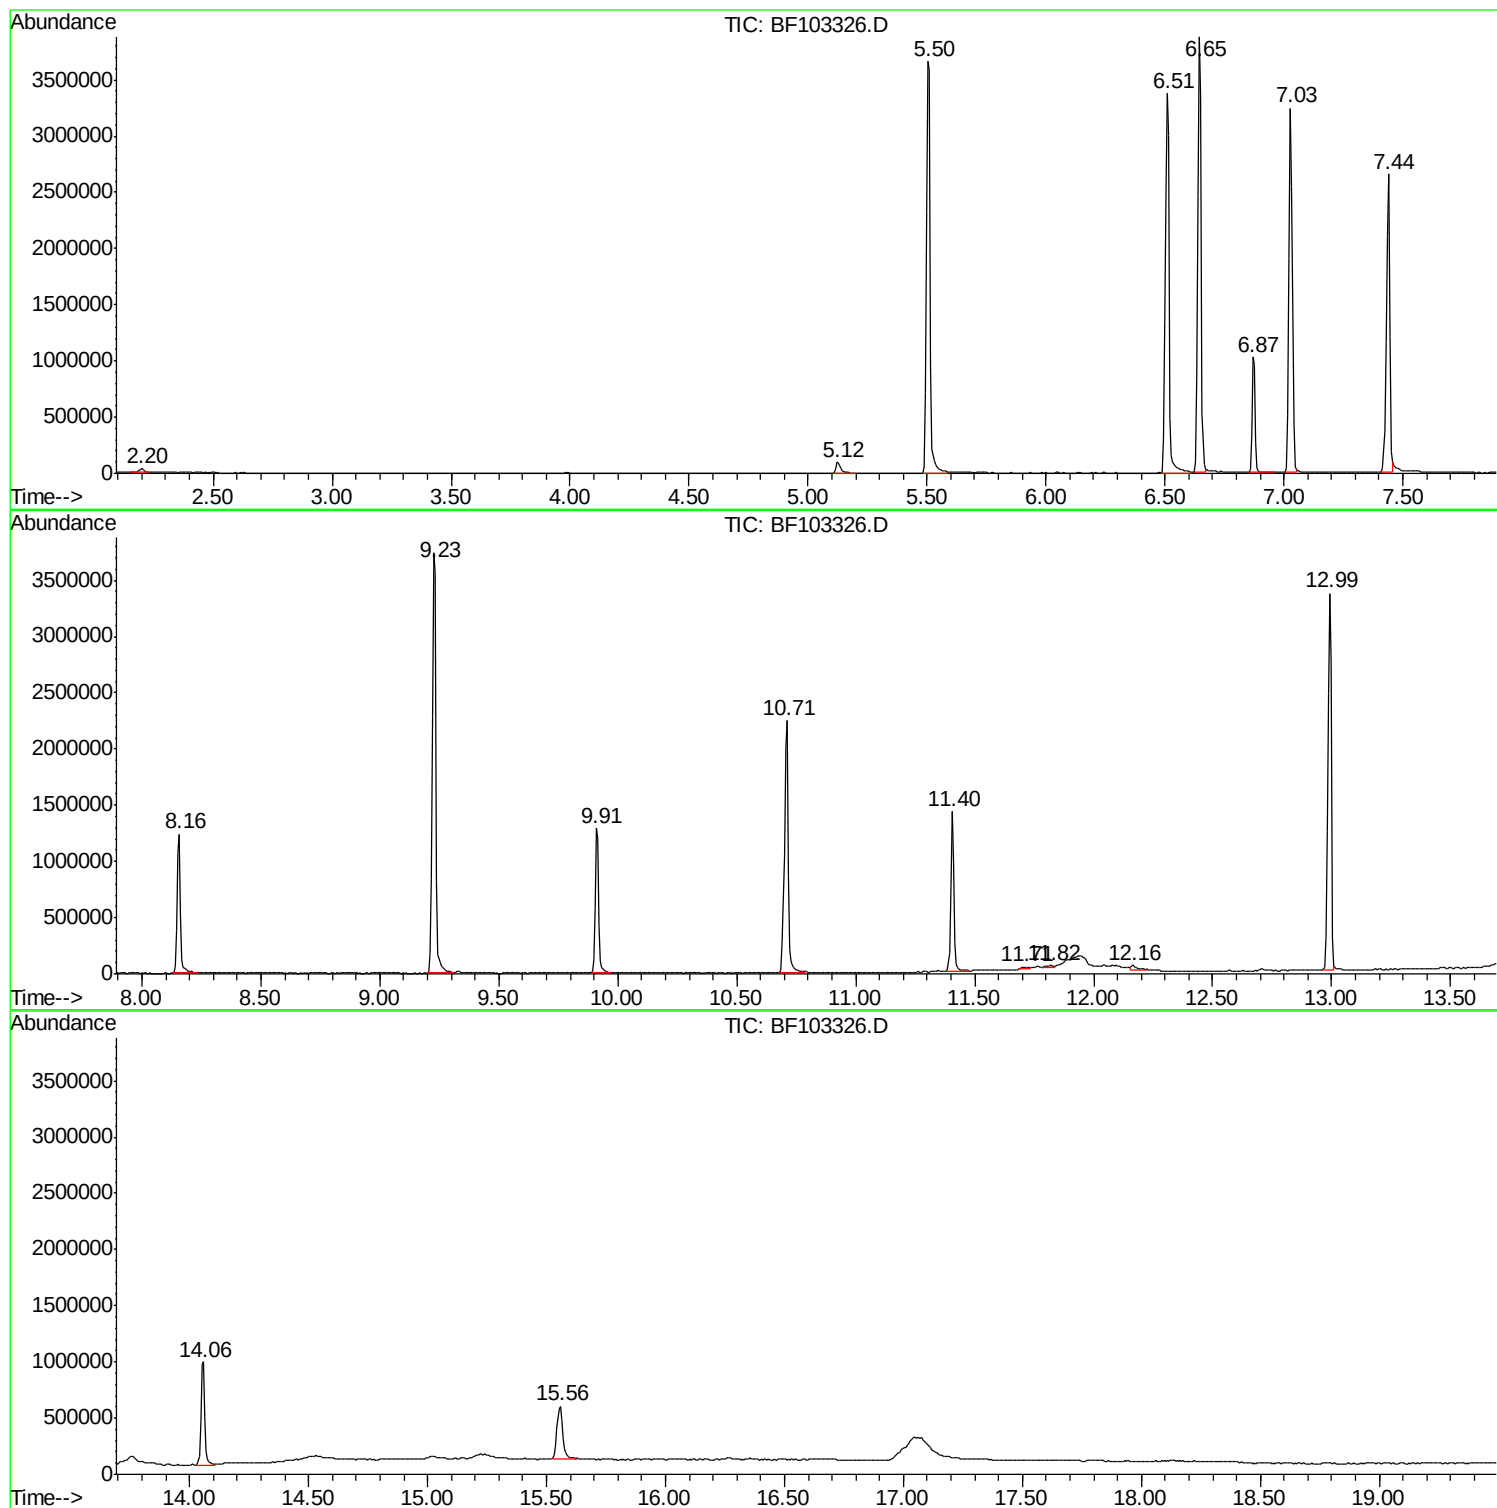

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF030118\
Data File : BF103326.D
Acq On : 1 Mar 2018 10:36
Operator : SJ/JU
Sample : PB106938BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB106938BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.12	2.90 ng	138622	1,4-Dichlorobenzene-d4	6.87

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28
3			2-Pentanol, 2,4-dimethyl-	116	C7H16O	000625-06-9	28
4			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
5			Acetone	58	C3H6O	000067-64-1	9

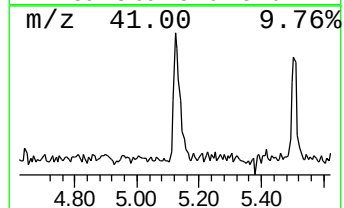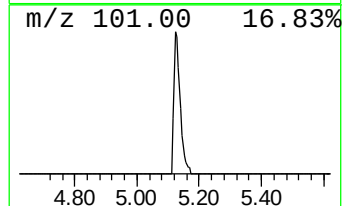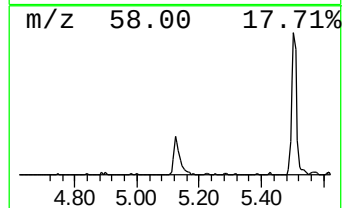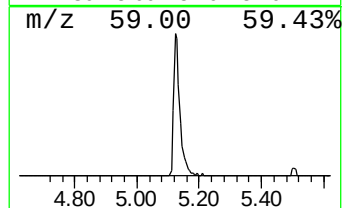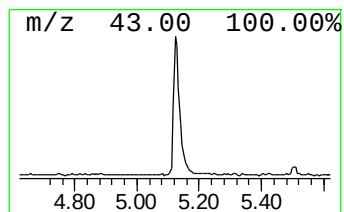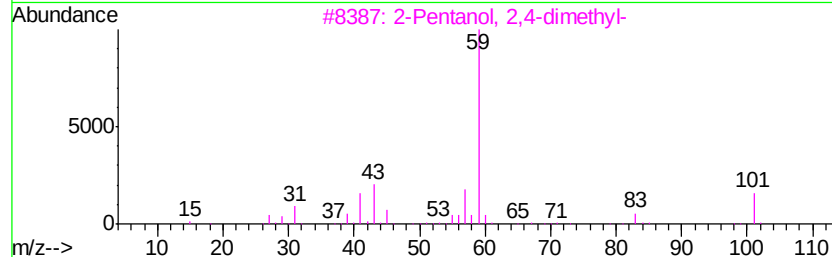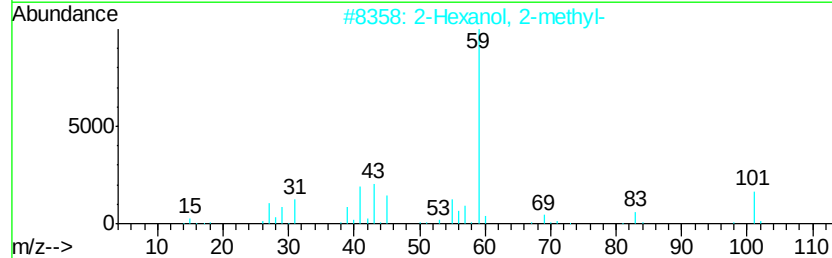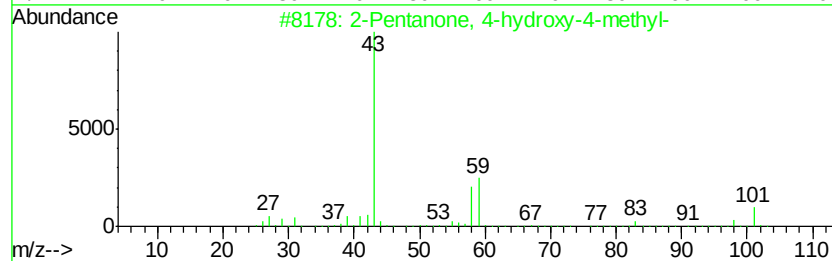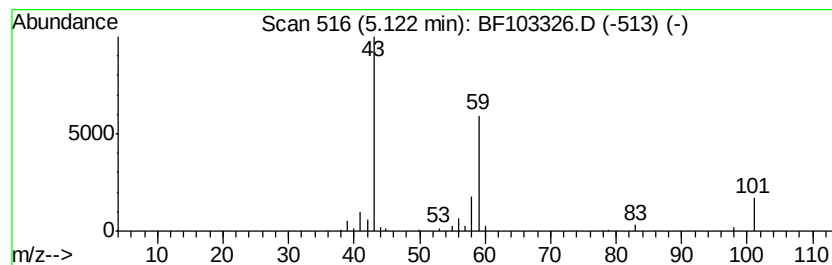

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030118\
Data File : BF103326.D
Acq On : 1 Mar 2018 10:36
Operator : SJ/JU
Sample : PB106938BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB106938BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	82.63 ng	3950020	1,4-Dichlorobenzene-d4	6.87

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

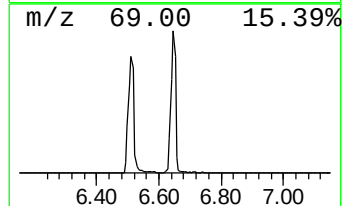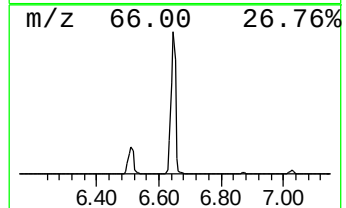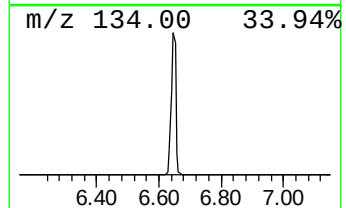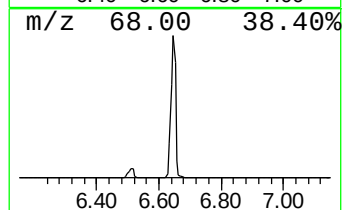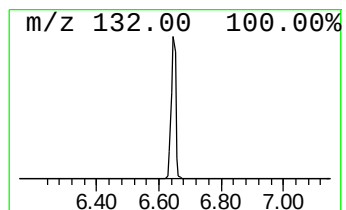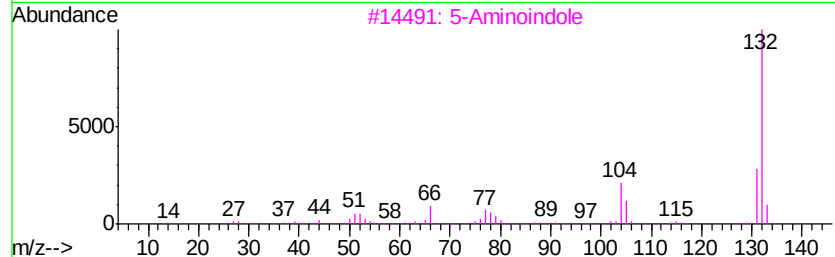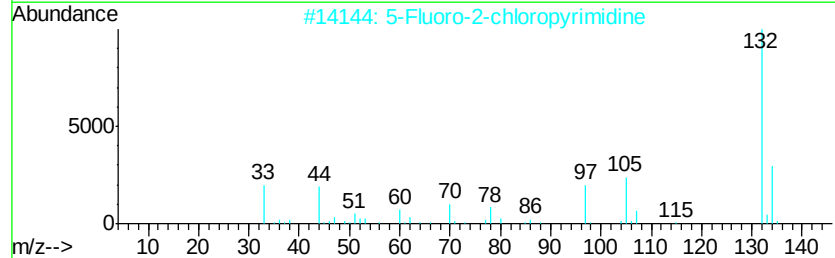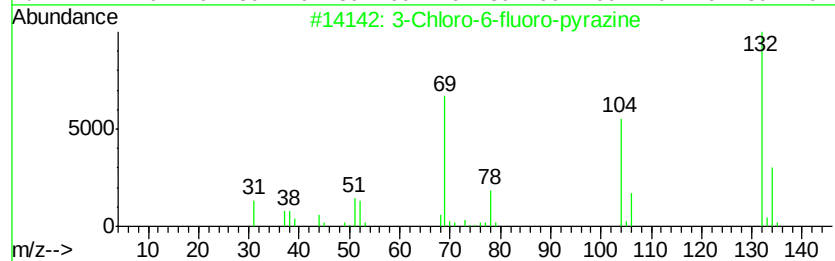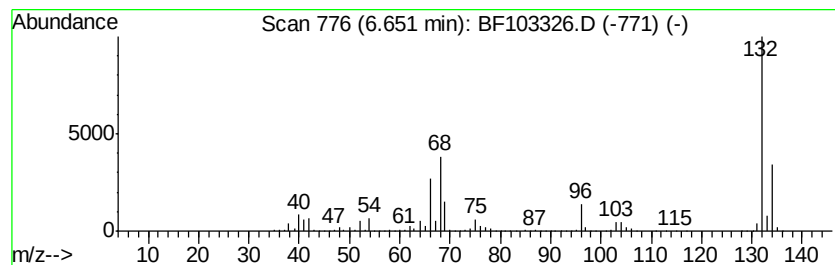

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF030118\
Data File : BF103326.D
Acq On : 1 Mar 2018 10:36
Operator : SJ/JU
Sample : PB106938BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB106938BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.12	2.9	ng	138622	1	6.87	956077	20.0
unknown6.65	6.65	82.6	ng	3950020	1	6.87	956077	20.0