


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030118\
 Data File : BF103323.D
 Acq On : 1 Mar 2018 8:45
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 27 17:05:20 2018

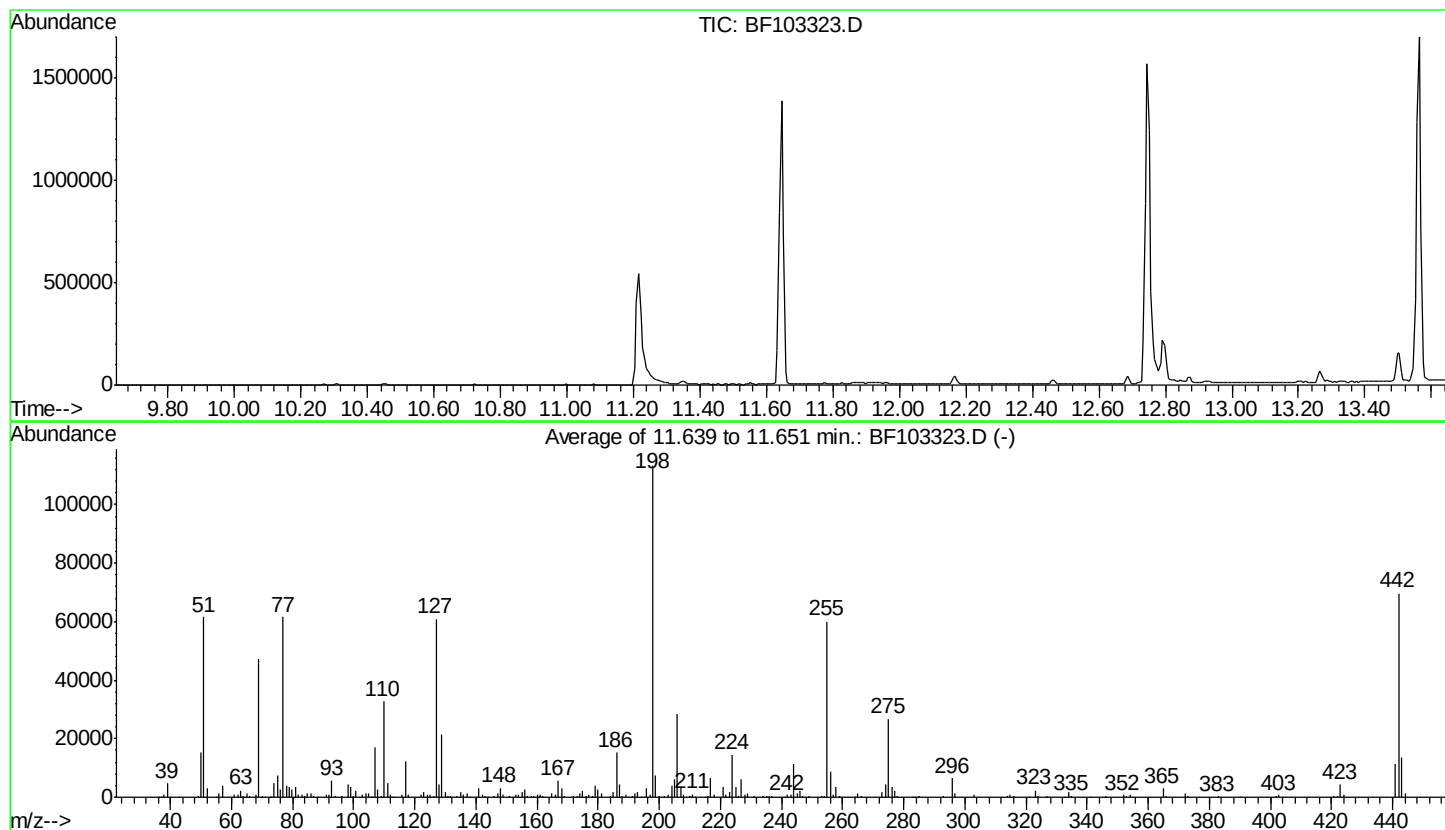

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	61498	PASS
68	69	0.00	2	1.8	867	PASS
69	198	0.00	100	41.7	47233	PASS
70	69	0.00	2	0.5	237	PASS
127	198	10	80	53.7	60821	PASS
197	198	0.00	2	0.8	855	PASS
198	198	100	100	100.0	113304	PASS
199	198	5	9	6.6	7494	PASS
275	198	10	60	23.8	26912	PASS
365	198	1	100	2.7	3059	PASS
441	443	0.01	100	85.3	11516	PASS
442	198	50	100	61.4	69600	PASS
443	442	15	24	19.4	13503	PASS