


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030118\
 Data File : BF103349.D
 Acq On : 1 Mar 2018 21:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 27 17:05:20 2018

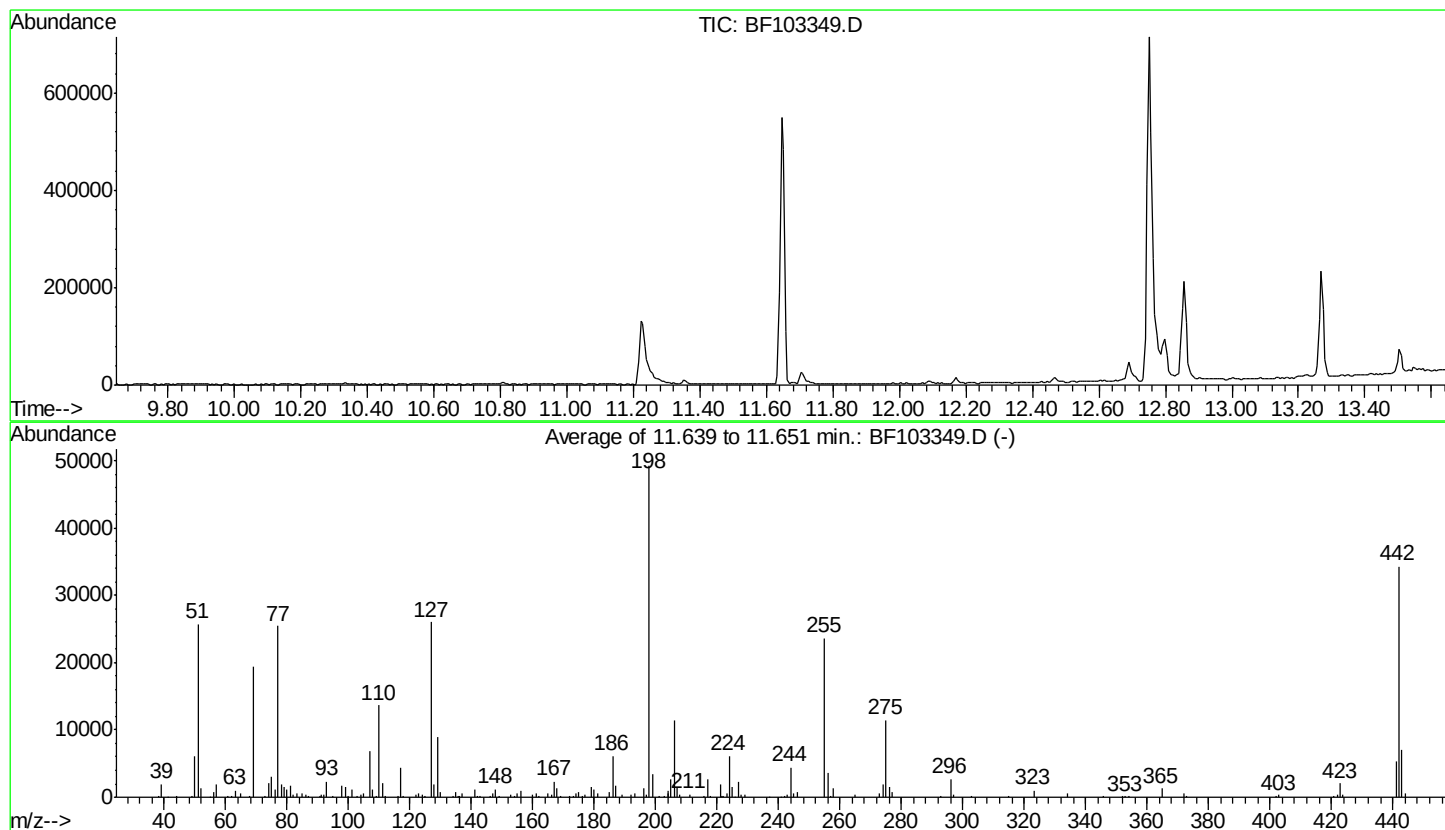

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.2	25738	PASS
68	69	0.00	2	0.7	140	PASS
69	198	0.00	100	39.5	19474	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.8	26005	PASS
197	198	0.00	2	0.9	451	PASS
198	198	100	100	100.0	49282	PASS
199	198	5	9	6.9	3380	PASS
275	198	10	60	23.3	11486	PASS
365	198	1	100	2.7	1319	PASS
441	443	0.01	100	76.1	5352	PASS
442	198	50	100	69.5	34266	PASS
443	442	15	24	20.5	7032	PASS