

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030121\
 Data File : BF123323.D
 Acq On : 1 Mar 2021 13:04
 Operator : JU/CG
 Sample : PB134865BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134865BL

Quant Time: Mar 01 13:51:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 16:08:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.851	152	148957	20.00	ng	0.00
21) Naphthalene-d8	8.133	136	606745	20.00	ng	-0.01
39) Acenaphthene-d10	9.892	164	312453	20.00	ng	-0.01
64) Phenanthrene-d10	11.386	188	578287	20.00	ng	0.00
76) Chrysene-d12	14.033	240	476917	20.00	ng	-0.01
86) Perylene-d12	15.509	264	432003	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.487	112	1336383	129.14	ng	0.01
7) Phenol-d6	6.487	99	1716672	122.10	ng	0.00
23) Nitrobenzene-d5	7.416	82	1159559	87.48	ng	-0.01
42) 2,4,6-Tribromophenol	10.686	330	401070	126.06	ng	-0.01
45) 2-Fluorobiphenyl	9.216	172	1804272	82.95	ng	0.00
79) Terphenyl-d14	12.980	244	1995888	80.47	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030121\
Data File : BF123323.D
Acq On : 1 Mar 2021 13:04
Operator : JU/CG
Sample : PB134865BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134865BL

Quant Time: Mar 01 13:51:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration




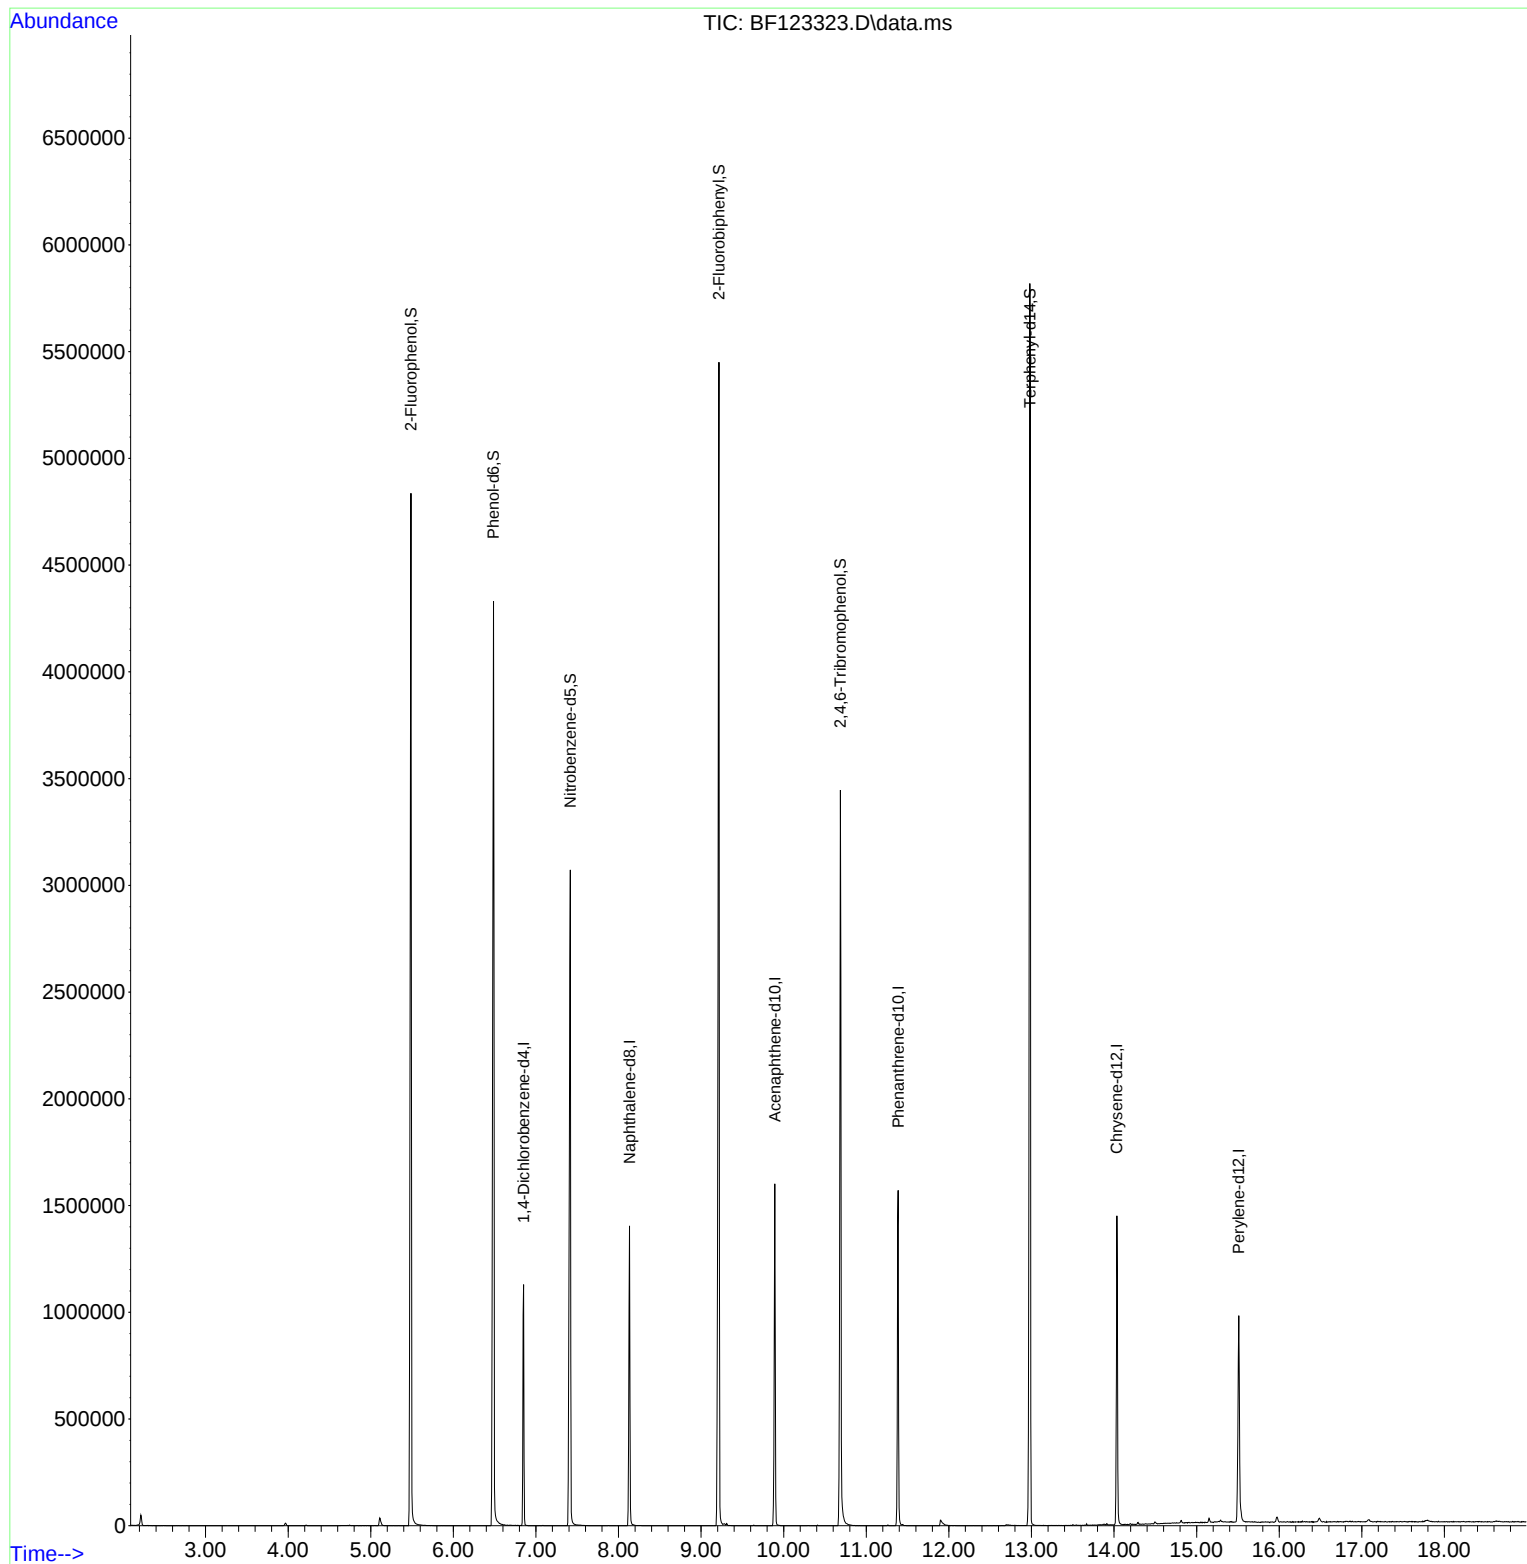


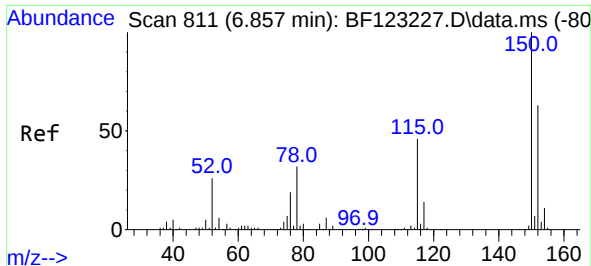

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.851 min Scan# 810
Delta R.T. -0.006 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04




Instrument :
BNA_F
ClientSampled :
PB134865BL


Tgt Ion:152 Resp: 148957
Ion Ratio Lower Upper
152 100
150 156.4 125.8 188.6
115 69.5 49.3 73.9

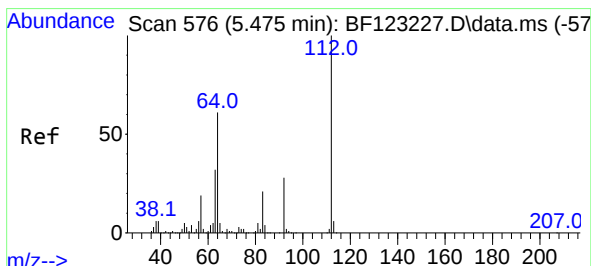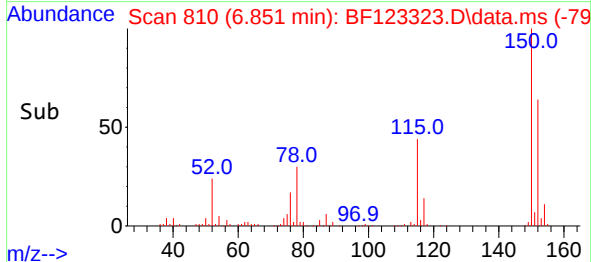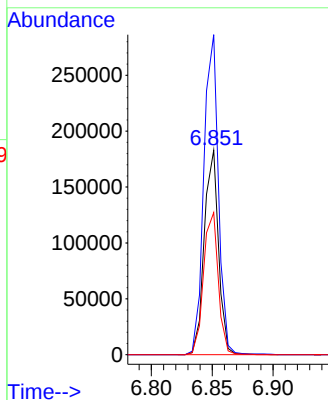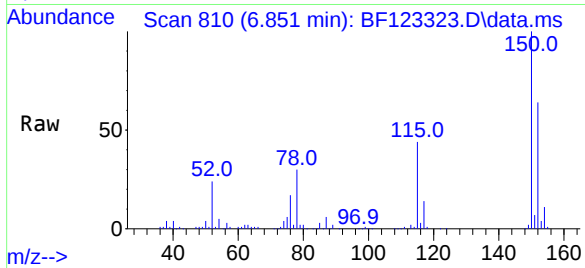

#5
2-Fluorophenol
Concen: 129.14 ng
RT: 5.487 min Scan# 578
Delta R.T. 0.012 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04

Tgt Ion:112 Resp: 1336383
Ion Ratio Lower Upper
112 100
64 65.5 46.9 70.3
63 35.0 24.5 36.7

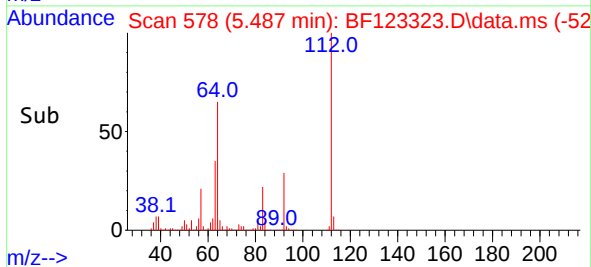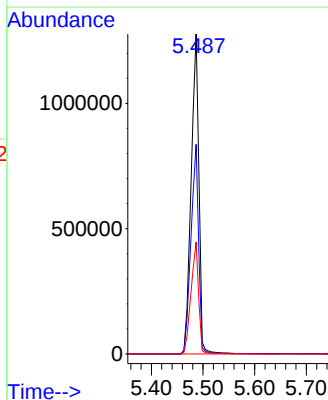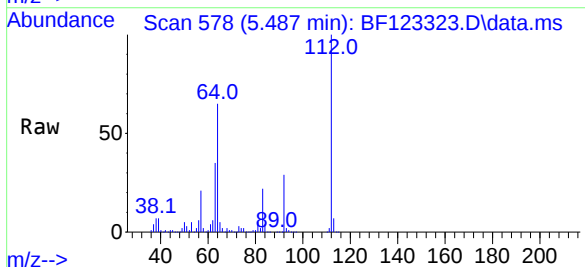




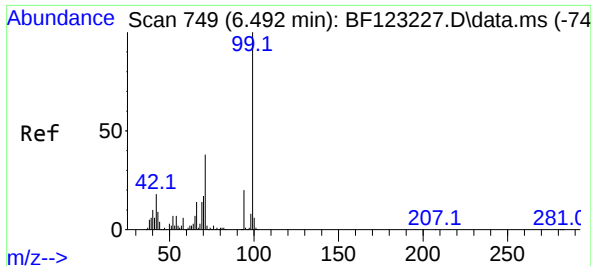


#7
Phenol-d6
Concen: 122.10 ng
RT: 6.487 min Scan# 748
Delta R.T. -0.006 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04

Instrument :
BNA_F
ClientSampleId :
PB134865BL

Tgt Ion: 99 Resp: 1716672




Ion	Ratio	Lower	Upper
99	100		
42	20.4	13.8	20.6
71	40.2	26.9	40.3

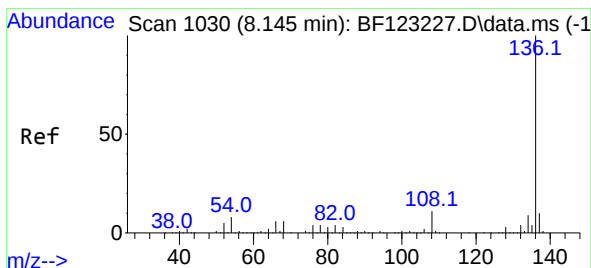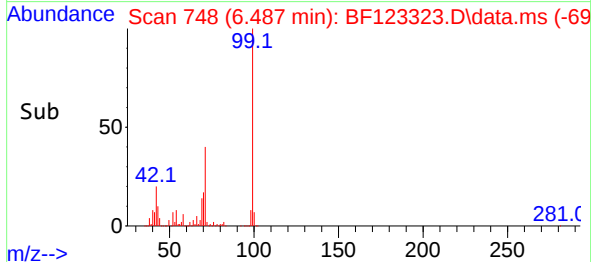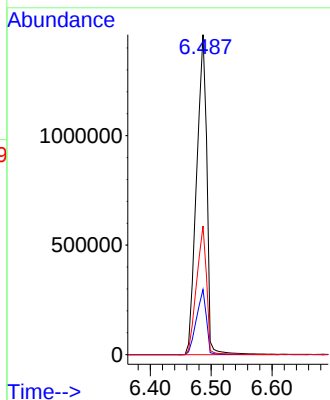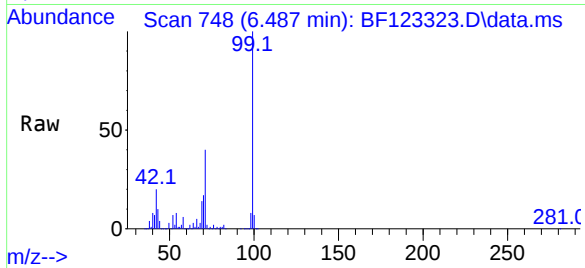


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.133 min Scan# 1028
Delta R.T. -0.012 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04

Tgt Ion: 136 Resp: 606745

Ion	Ratio	Lower	Upper
136	100		
137	10.4	8.8	13.2
54	8.2	5.5	8.3
68	5.9	4.6	6.8


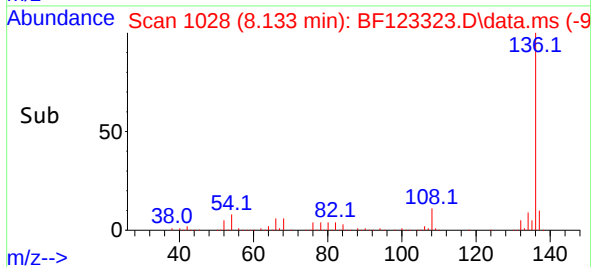
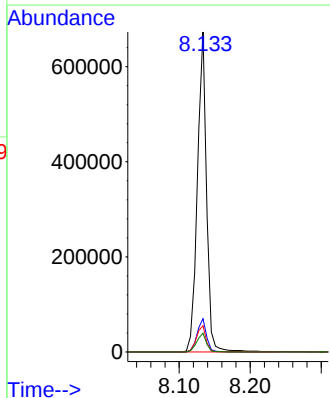
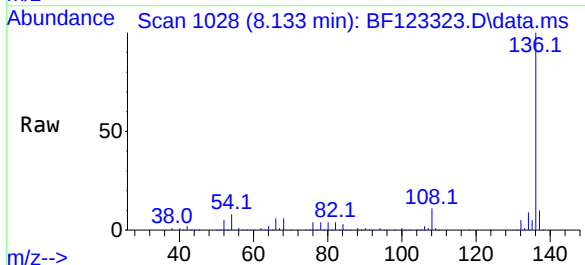


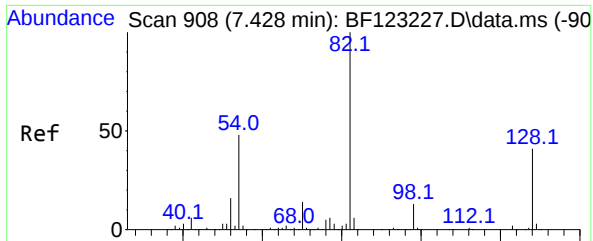

#23
Nitrobenzene-d5
Concen: 87.48 ng
RT: 7.416 min Scan# 906
Delta R.T. -0.012 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04




Instrument :
BNA_F
ClientSampleId :
PB134865BL


Tgt Ion: 82 Resp: 1159559
Ion Ratio Lower Upper
82 100
128 40.0 37.0 55.4
54 50.3 38.4 57.6

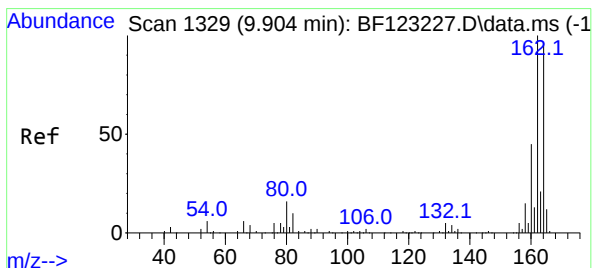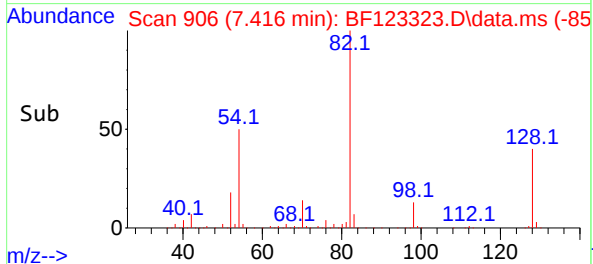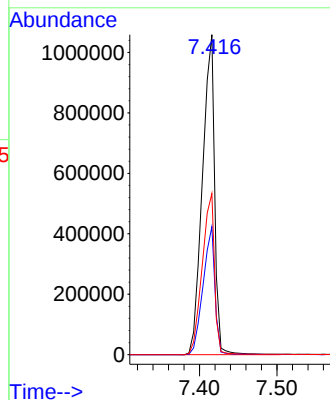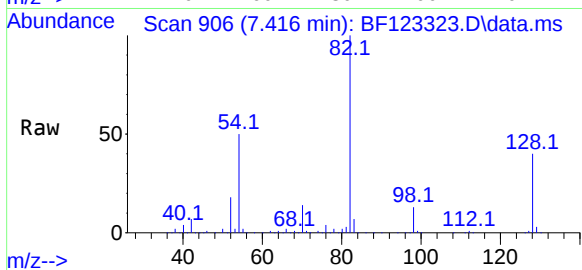

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.892 min Scan# 1327
Delta R.T. -0.012 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04

Tgt Ion:164 Resp: 312453
Ion Ratio Lower Upper
164 100
162 102.1 80.8 121.2
160 45.6 35.4 53.0


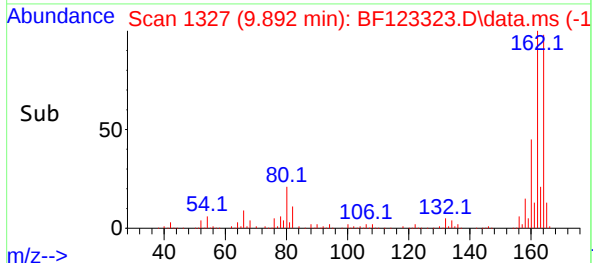
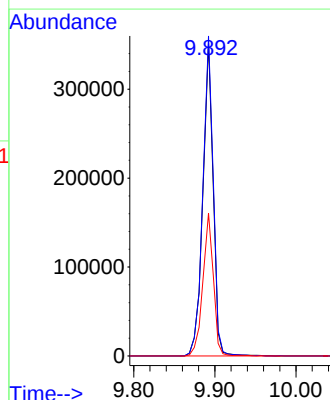
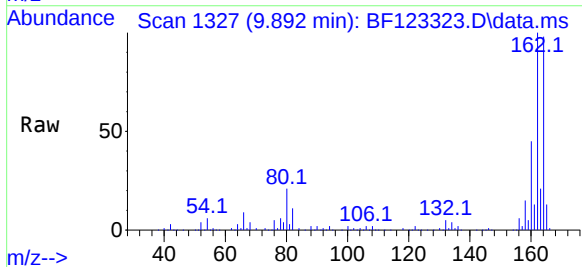


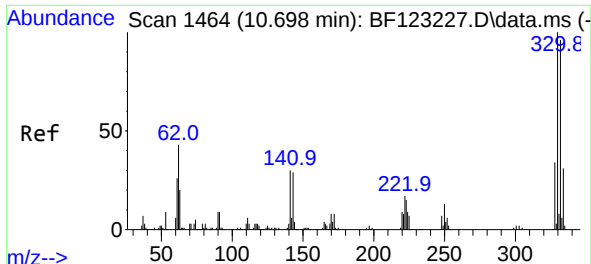

#42
2,4,6-Tribromophenol
Concen: 126.06 ng
RT: 10.686 min Scan# 1462
Delta R.T. -0.012 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04




Instrument :
BNA_F
ClientSampleId :
PB134865BL


Tgt Ion:330 Resp: 401070
Ion Ratio Lower Upper
330 100
332 96.1 77.5 116.3
141 41.7 23.8 35.8#

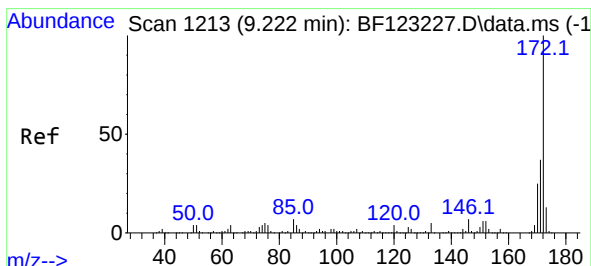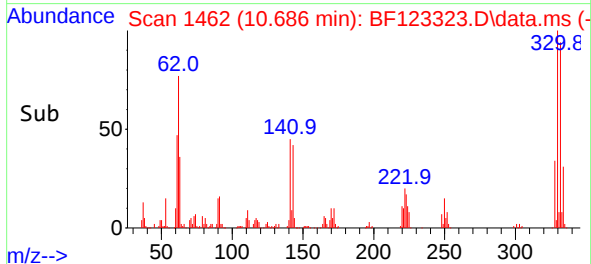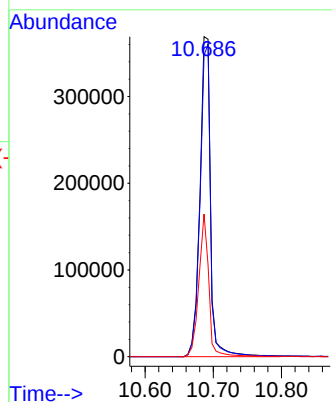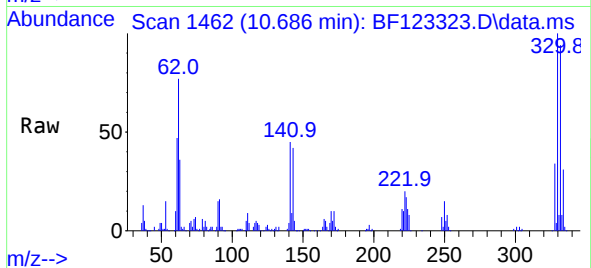

#45
2-Fluorobiphenyl
Concen: 82.95 ng
RT: 9.216 min Scan# 1212
Delta R.T. -0.006 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04

Tgt Ion:172 Resp: 1804272
Ion Ratio Lower Upper
172 100
171 36.7 29.6 44.4
170 24.3 19.5 29.3


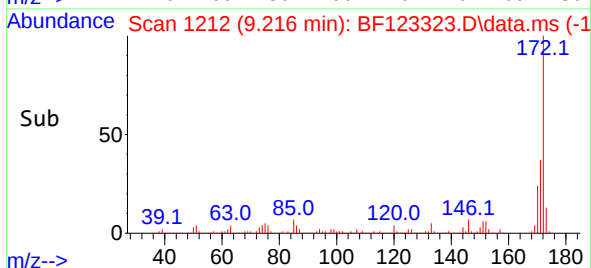
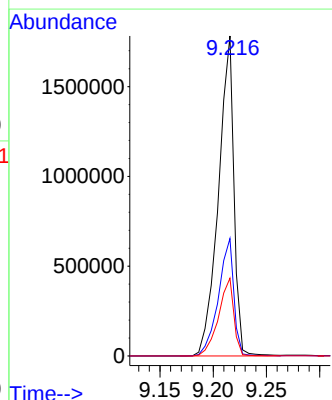
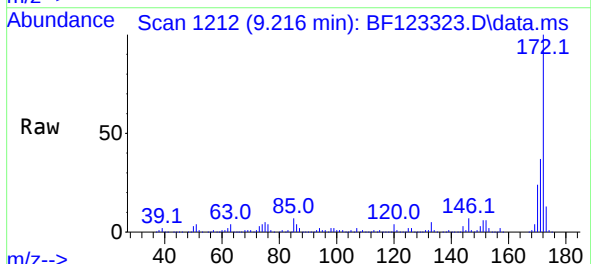


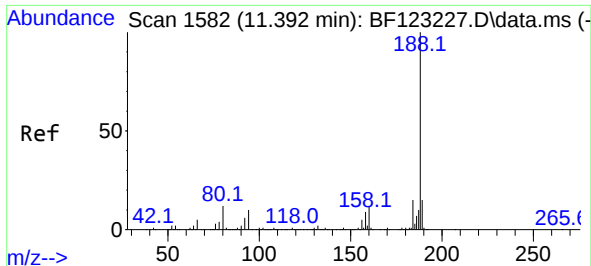

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.386 min Scan# 1581
Delta R.T. -0.006 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04




Instrument :
BNA_F
ClientSampleId :
PB134865BL


Tgt Ion:188 Resp: 578287
Ion Ratio Lower Upper
188 100
94 9.1 7.4 11.2
80 10.5 8.2 12.4

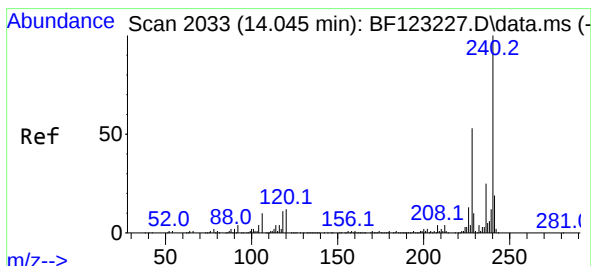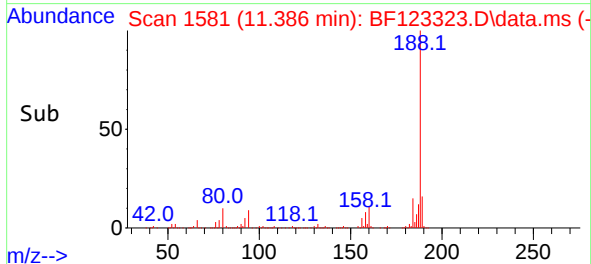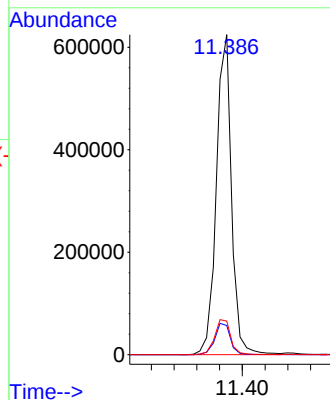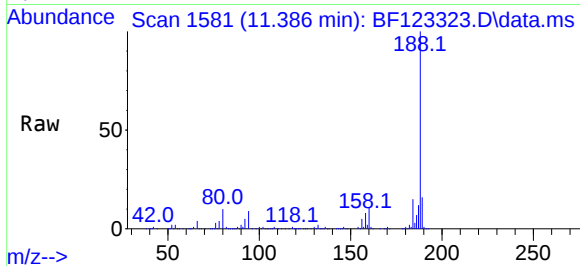

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.033 min Scan# 2031
Delta R.T. -0.012 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04


Tgt Ion:240 Resp: 476917
Ion Ratio Lower Upper
240 100
120 11.9 8.6 12.8
236 25.2 20.3 30.5

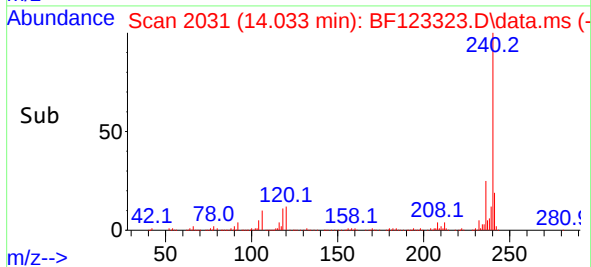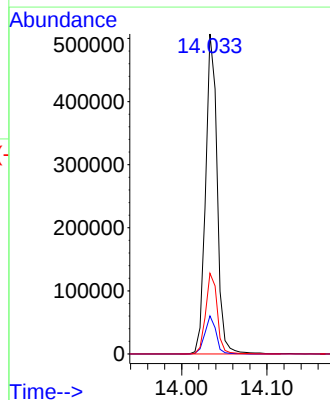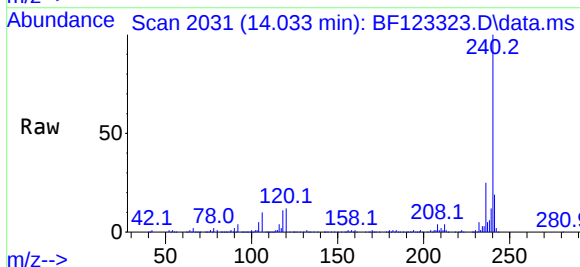



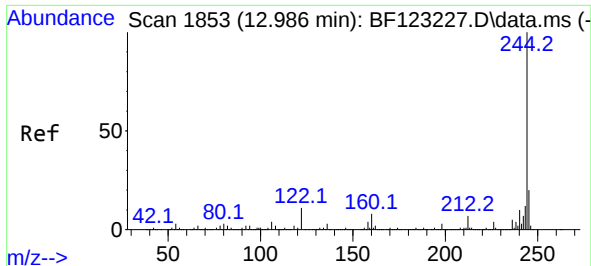


#79
Terphenyl-d14
Concen: 80.47 ng
RT: 12.980 min Scan# 1852
Delta R.T. -0.006 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04


Instrument :
BNA_F
ClientSampleId :
PB134865BL

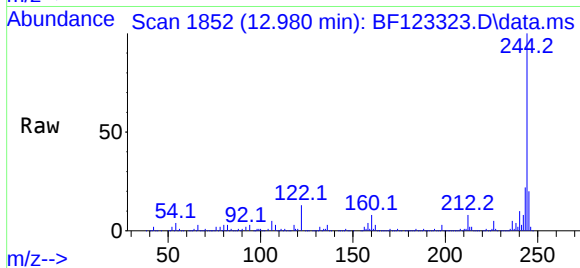

Tgt Ion:244 Resp: 1995888
Ion Ratio Lower Upper
244 100
212 7.5 5.7 8.5
122 12.6 8.3 12.5#

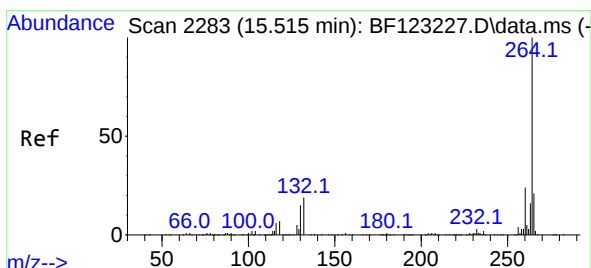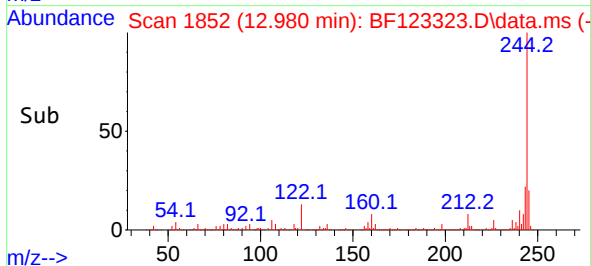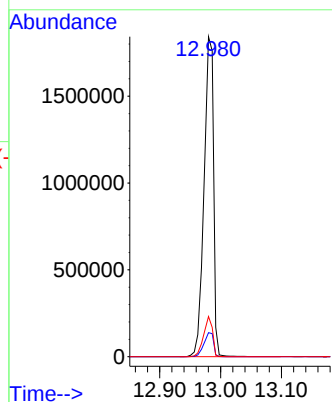

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.509 min Scan# 2282
Delta R.T. -0.006 min
Lab File: BF123323.D
Acq: 1 Mar 2021 13:04

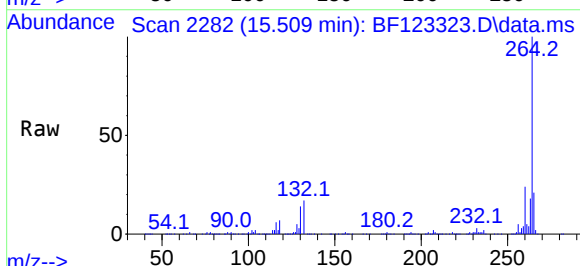

Tgt Ion:264 Resp: 432003
Ion Ratio Lower Upper
264 100
260 24.1 18.6 28.0
265 21.5 17.0 25.6

