


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030121\
 Data File : BF123318.D
 Acq On : 1 Mar 2021 9:19
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 16:08:53 2021

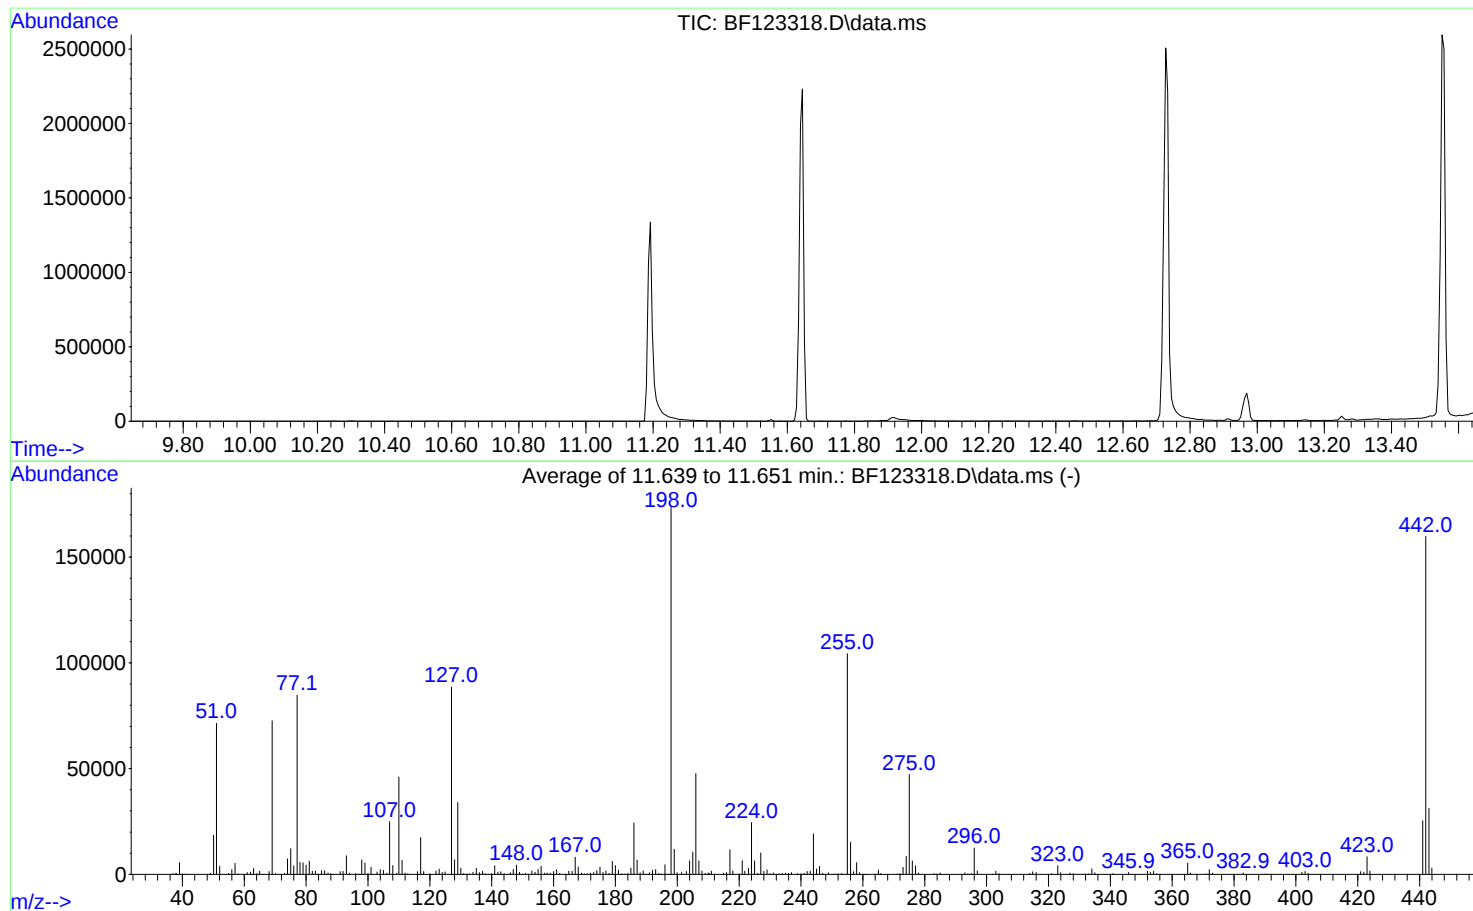




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	71456	PASS
68	69	0.00	2	1.9	1359	PASS
69	198	0.00	100	41.8	72624	PASS
70	69	0.00	2	0.5	362	PASS
127	198	10	80	50.9	88597	PASS
197	198	0.00	2	0.1	189	PASS
198	198	100	100	100.0	173941	PASS
199	198	5	9	6.8	11852	PASS
275	198	10	60	27.2	47245	PASS
365	198	1	100	3.1	5405	PASS
441	198	0.01	100	14.6	25373	PASS
442	442	50	100	100.0	159776	PASS
443	442	15	24	19.5	31163	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030121\
 Data File : BF123318.D
 Acq On : 1 Mar 2021 9:19
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 01 10:05:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 16:08:53 2021
 Response via : Initial Calibration

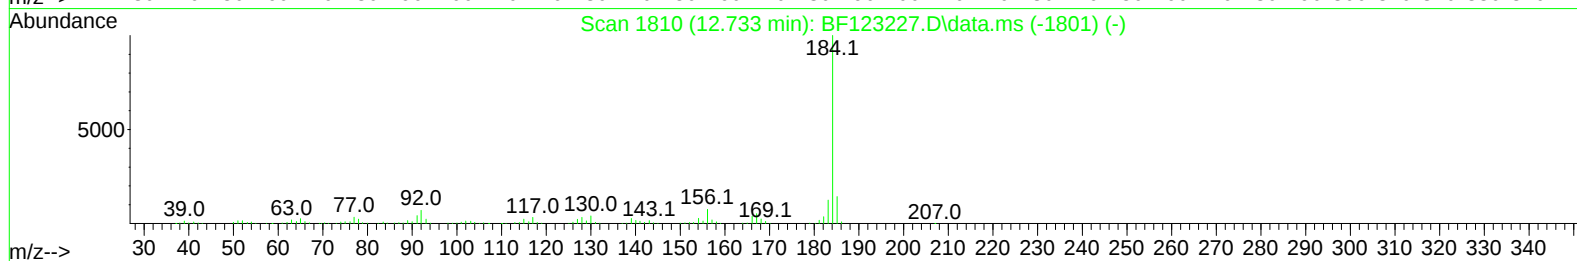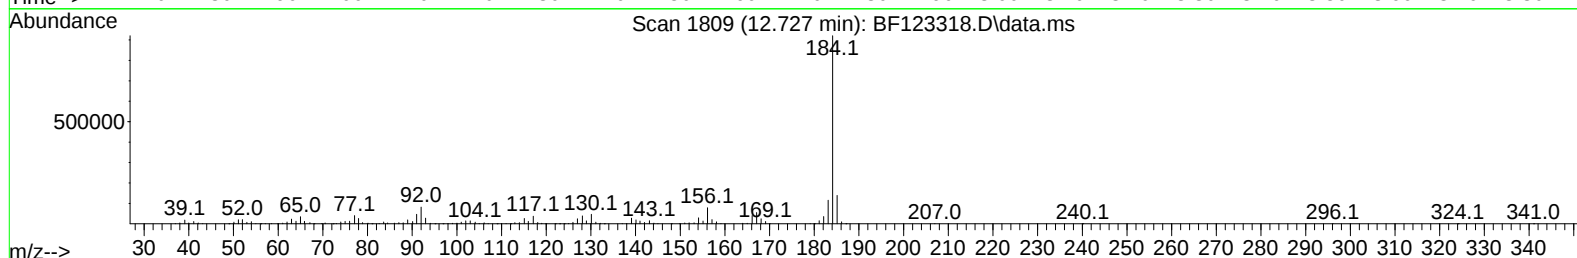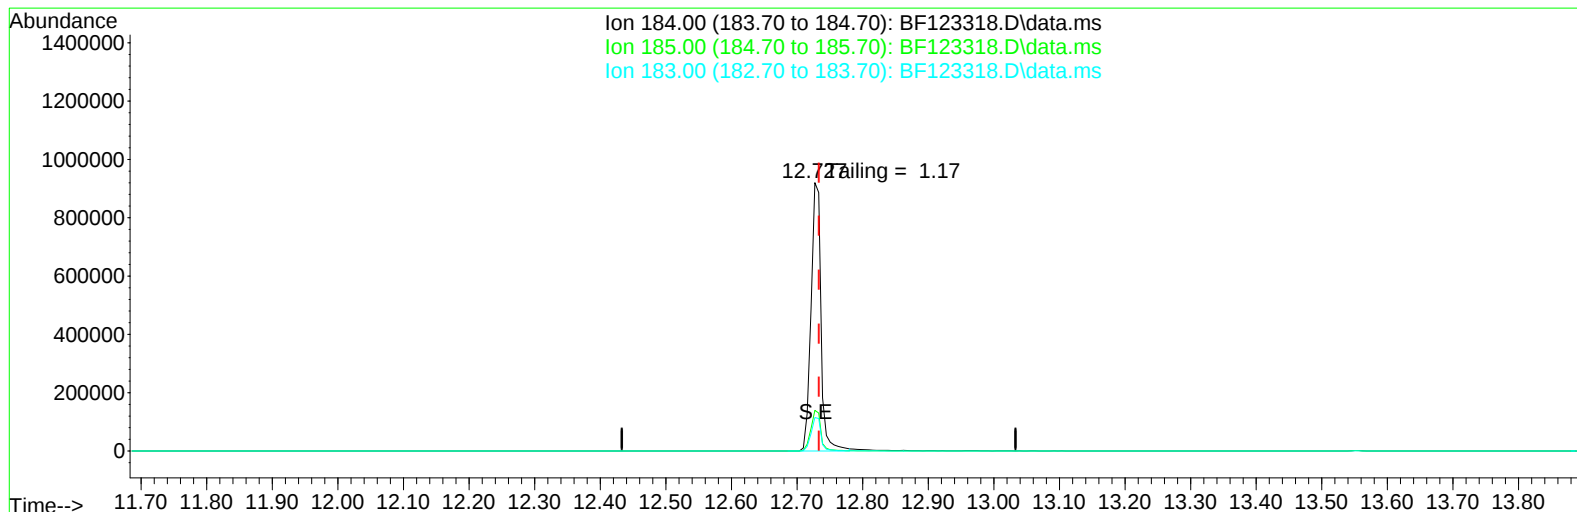

TIC: BF123318.D\data.ms

(77) Benzidine

12.727min (-0.006) 0.00 ng




response 995542

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.13
183.00	12.10	12.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030121\
Data File : BF123318.D
Acq On : 1 Mar 2021 9:19
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 01 10:05:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

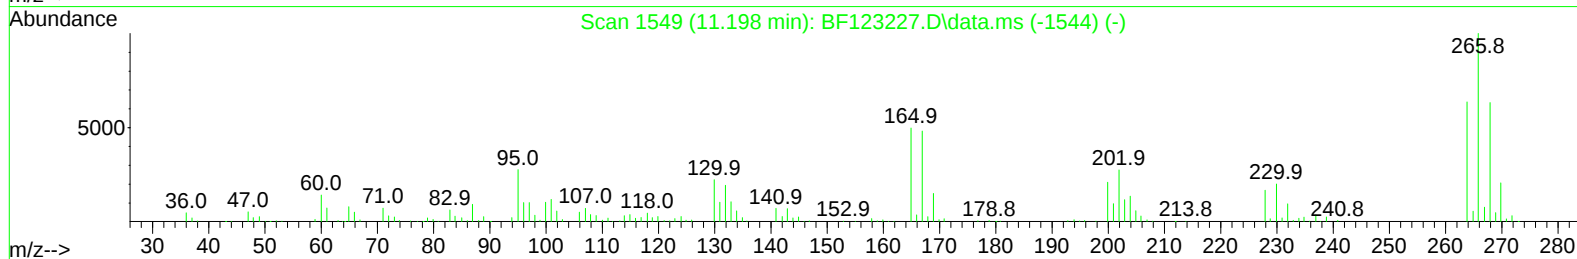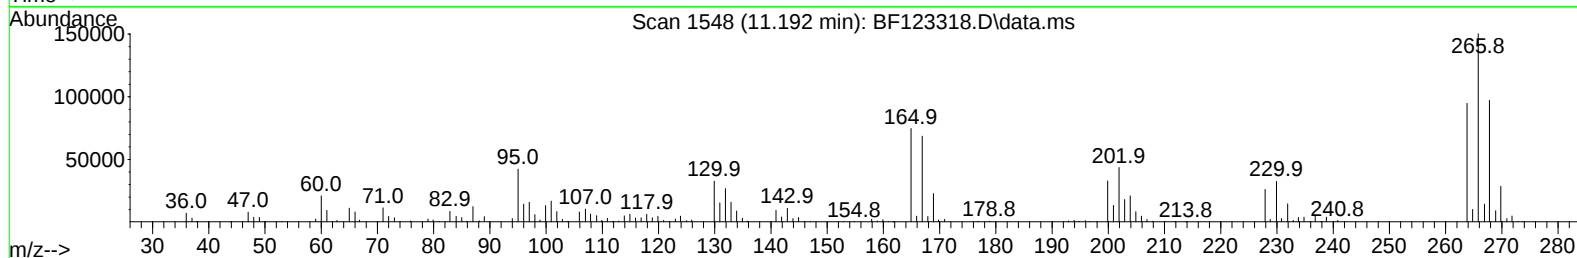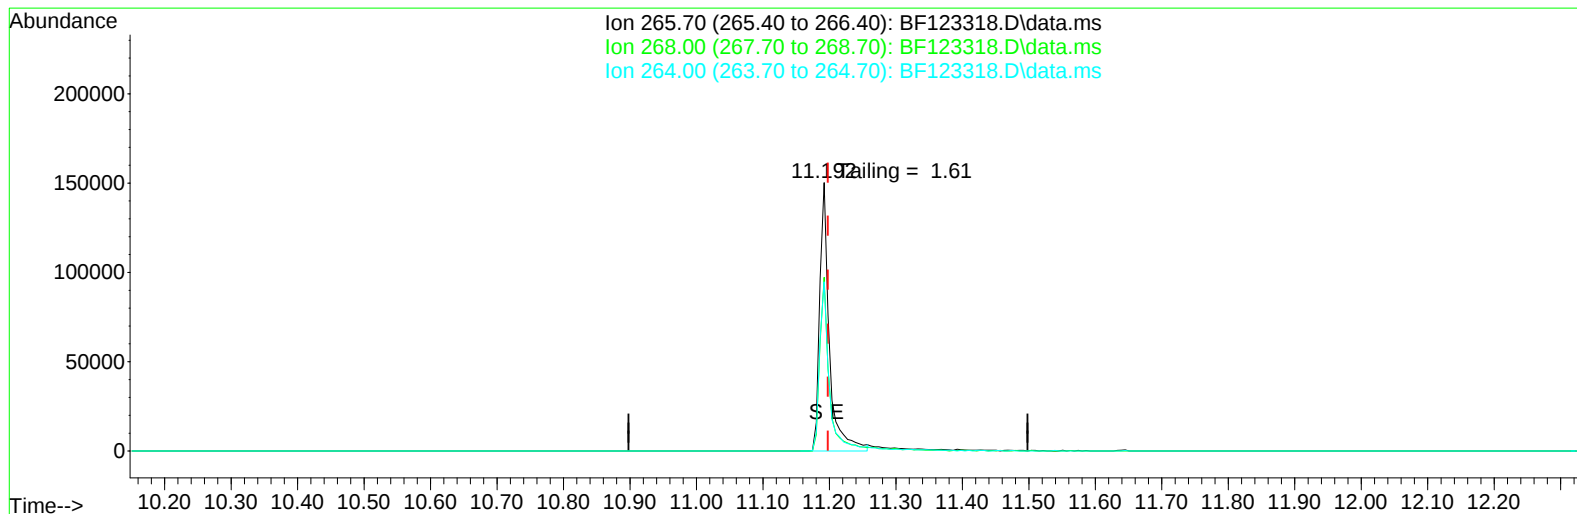

TIC: BF123318.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 22429.33 ng

response 160368

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.71
264.00	62.30	63.04
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
3/1/2021	BNA_F	<u>BF123318.D</u>
Compound Name	Response	Retention Time
DDT	440081	13.55
DDD	5411	13.25
DDE	1862	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7273	447354	1.63