
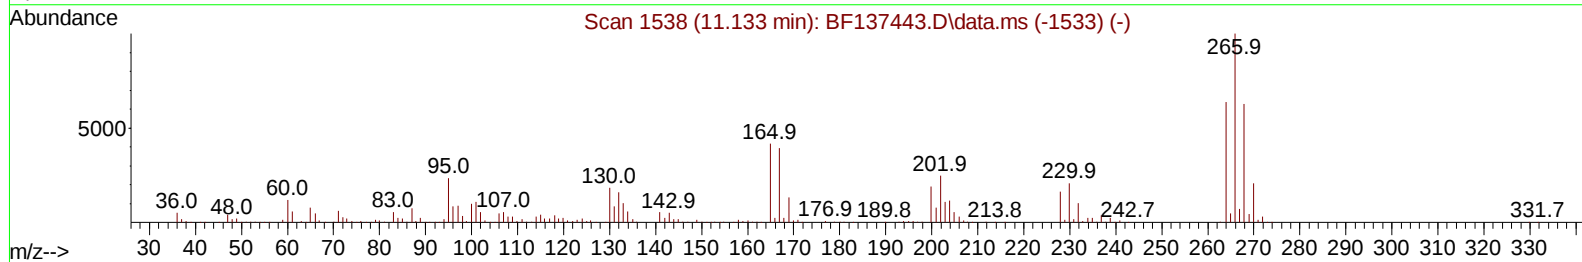
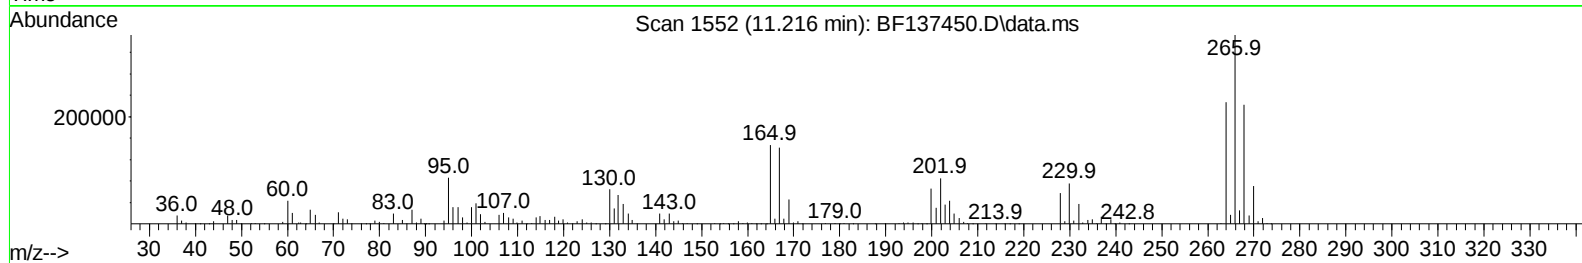


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030124\
Data File : BF137450.D
Acq On : 01 Mar 2024 09:51
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 11:40:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 11:26:52 2024
Response via : Initial Calibration

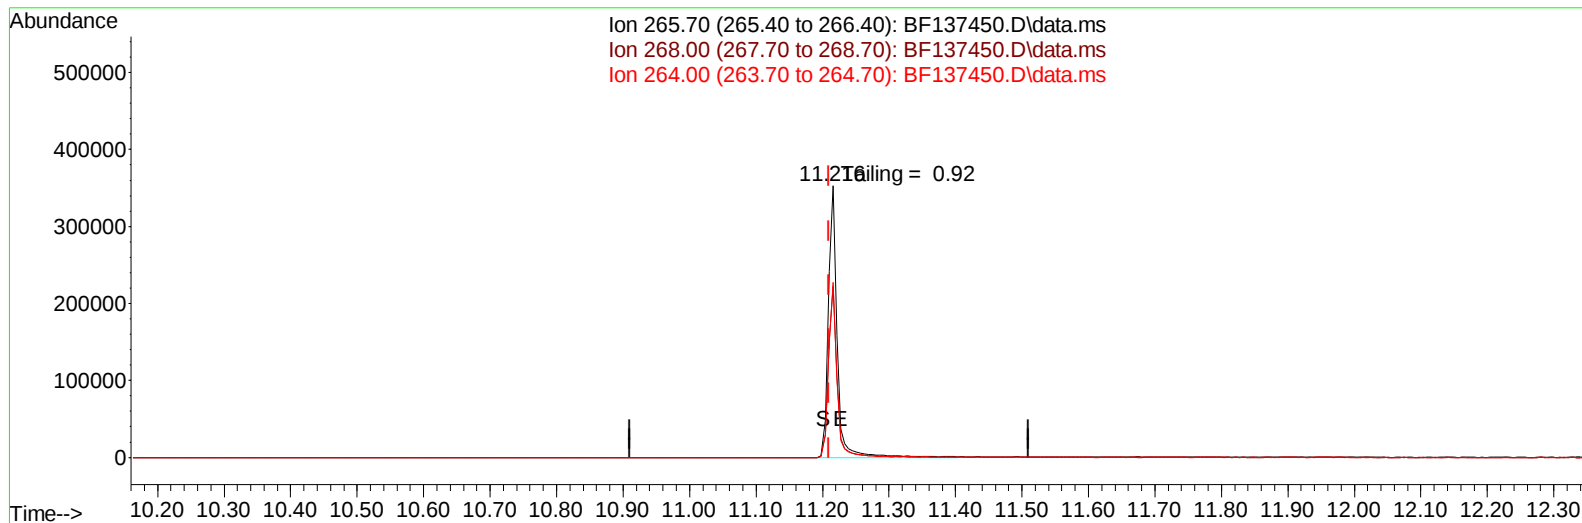

TIC: BF137450.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 90926.27 ng

response 327737

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.12
264.00	63.60	64.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030124\
Data File : BF137450.D
Acq On : 01 Mar 2024 09:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 11:40:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 11:26:52 2024
Response via : Initial Calibration

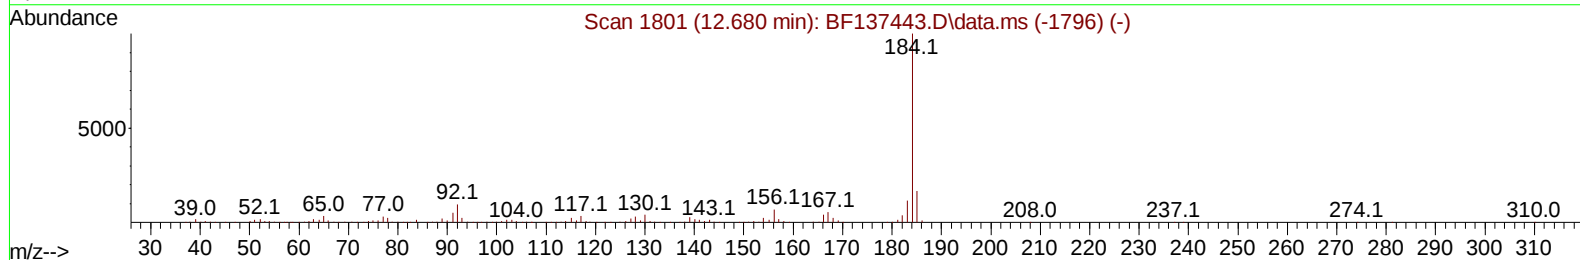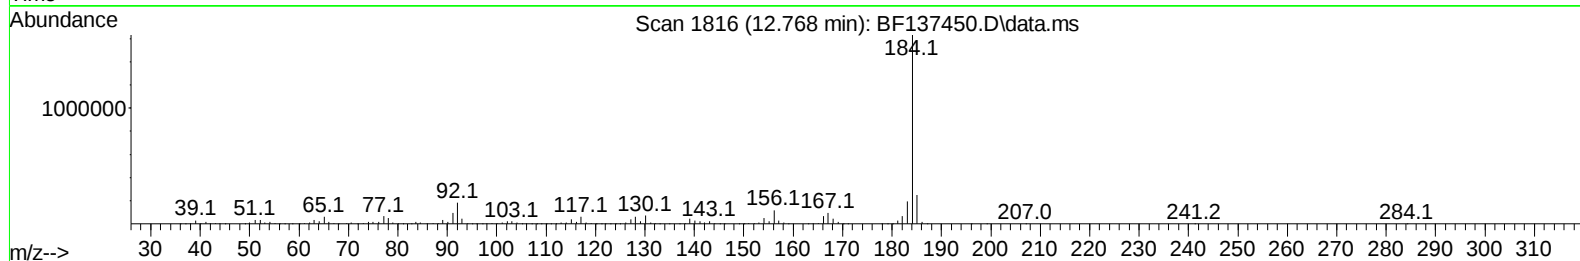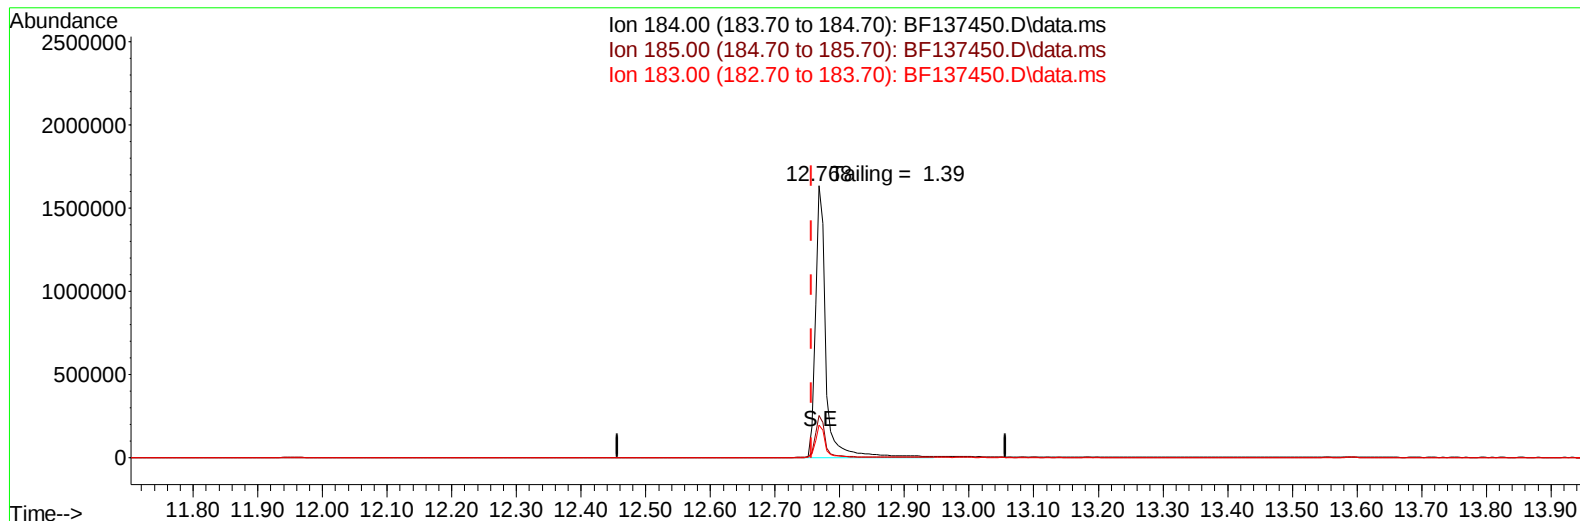

TIC: BF137450.D\data.ms

(77) Benzidine**12.768min (+ 0.012) 25947.74 ng****response 1874519**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	15.37
183.00	11.60	11.84
0.00	0.00	0.00