


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030124\
Data File : BF137450.D
Acq On : 01 Mar 2024 09:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 04 00:26:53 2024

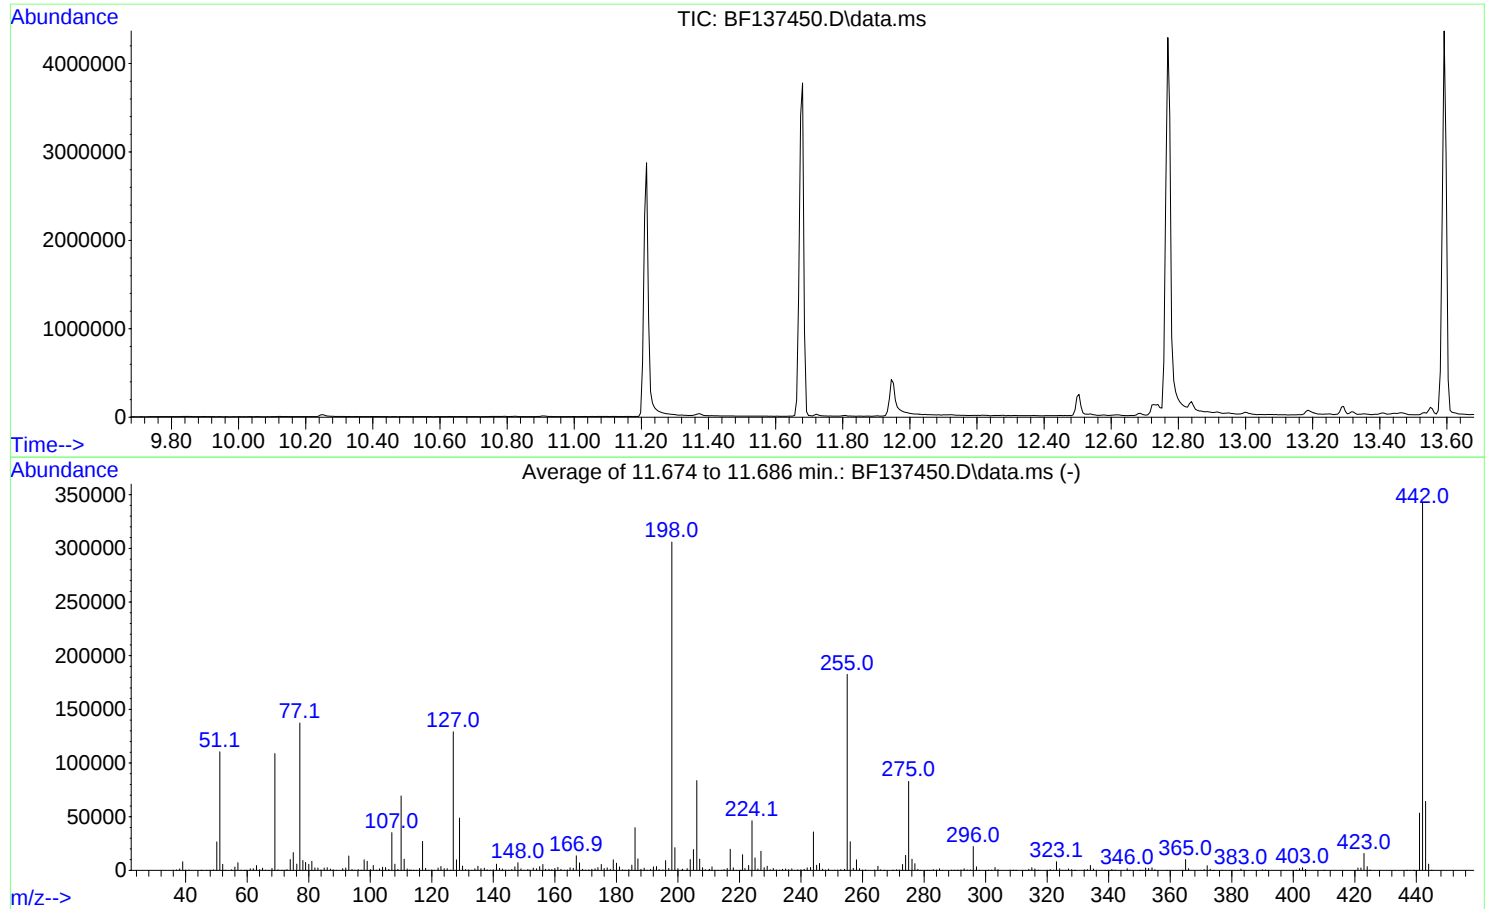




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	110483	PASS
68	69	0.00	2	1.7	1830	PASS
69	198	0.00	100	35.6	108845	PASS
70	69	0.00	2	0.6	641	PASS
127	198	10	80	42.2	129136	PASS
197	198	0.00	2	0.6	1768	PASS
198	198	100	100	100.0	305832	PASS
199	198	5	9	6.9	21206	PASS
275	198	10	60	27.1	82968	PASS
365	198	1	100	3.3	10192	PASS
441	198	0.01	100	17.5	53416	PASS
442	442	50	100	100.0	342720	PASS
443	442	15	24	18.7	64245	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030124\
 Data File : BF137450.D
 Acq On : 01 Mar 2024 09:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 01 11:40:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 01 11:26:52 2024
 Response via : Initial Calibration

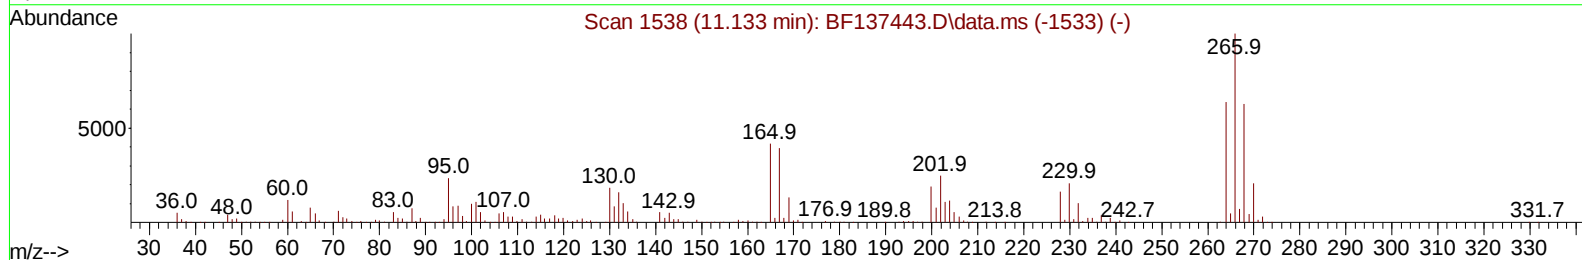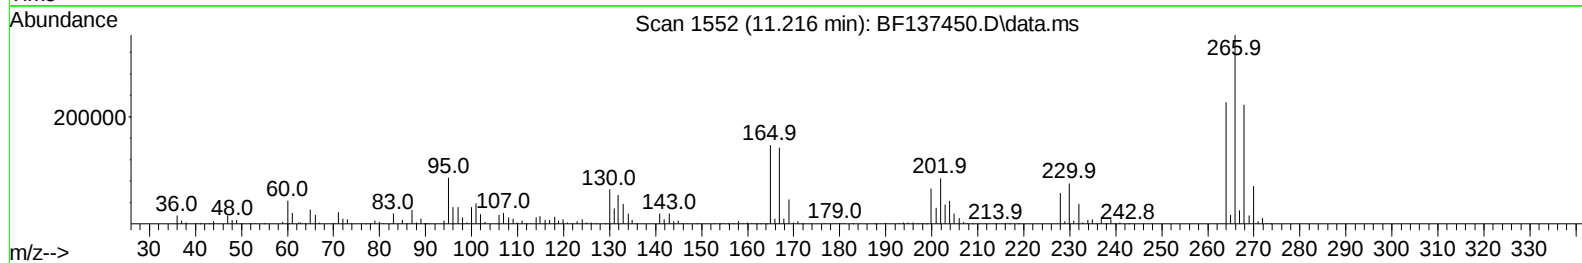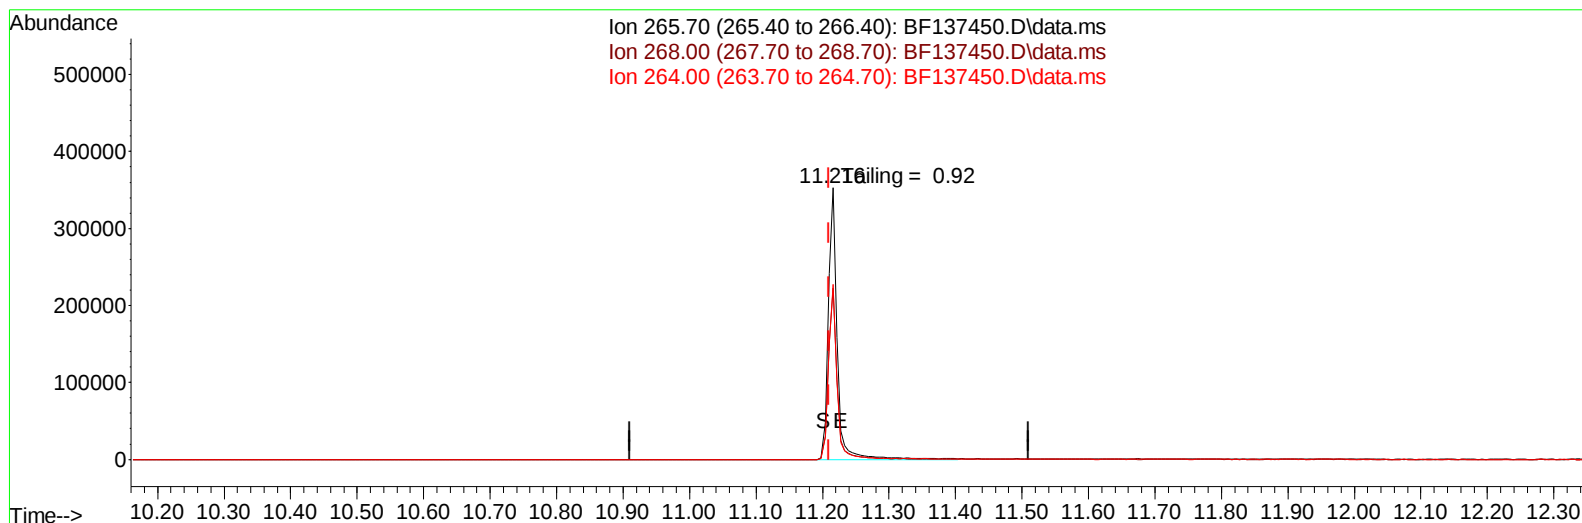

TIC: BF137450.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 90926.27 ng




response 327737

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.12
264.00	63.60	64.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030124\
 Data File : BF137450.D
 Acq On : 01 Mar 2024 09:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 01 11:40:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 01 11:26:52 2024
 Response via : Initial Calibration

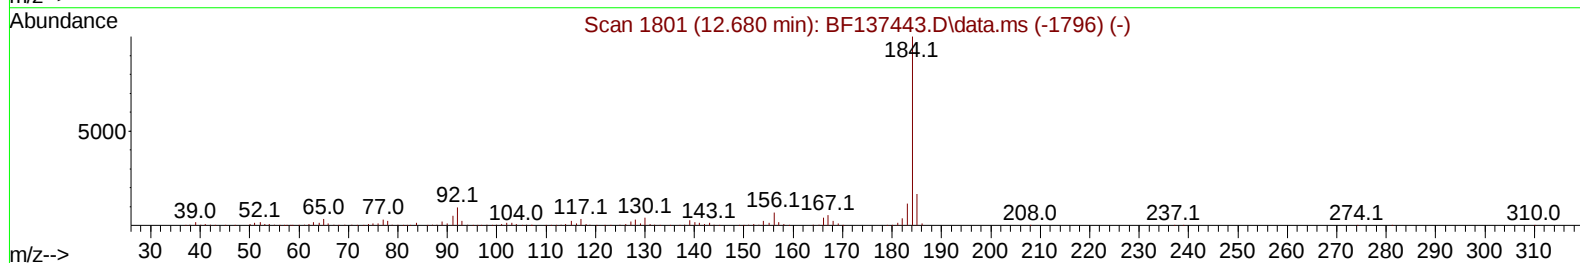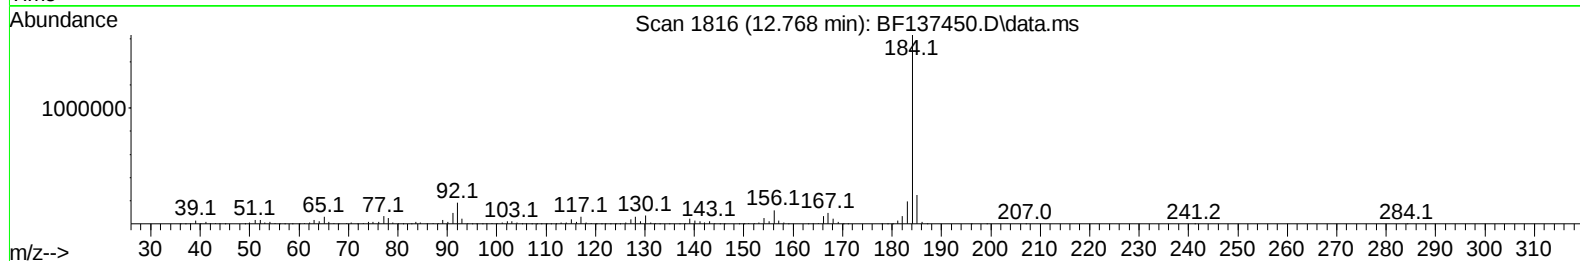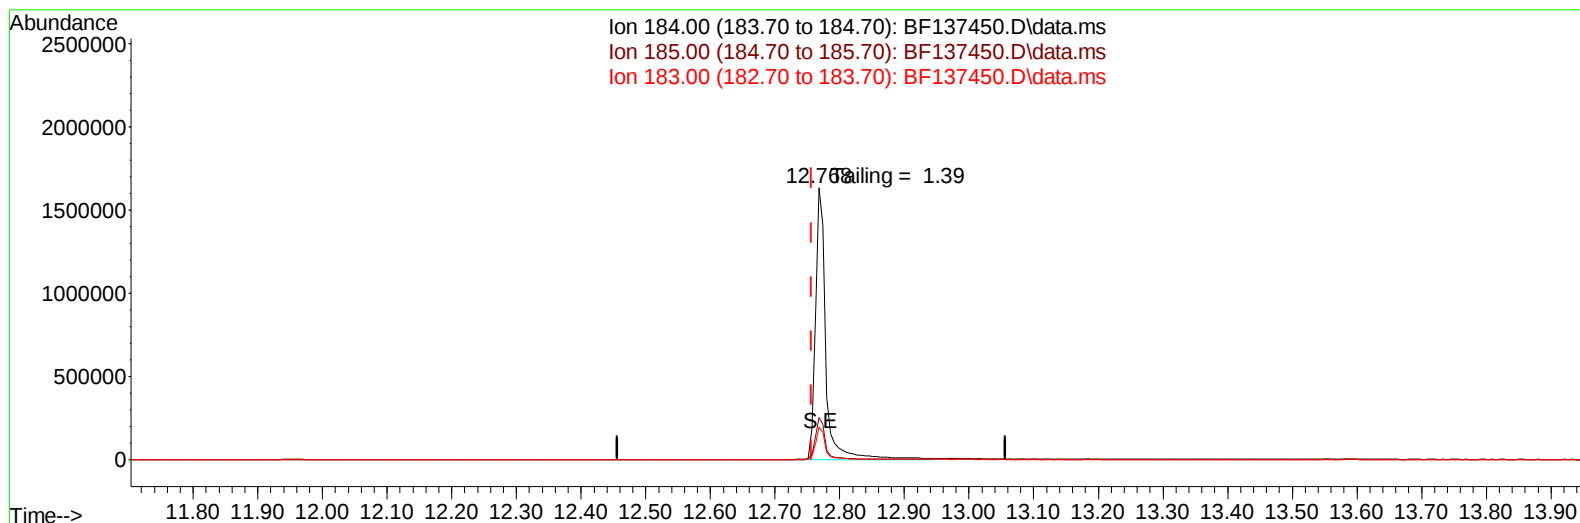

TIC: BF137450.D\data.ms

(77) Benzidine

12.768min (+ 0.012) 25947.74 ng

response 1874519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	15.37
183.00	11.60	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/1/2024	BNA_F	<u>BF137450.D</u>
Compound Name	Response	Retention Time
DDT	717728	13.592
DDD	23443	13.292
DDE	1371	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24814	742542	3.34

Instrument :
BNA_F
ClientSampleId :
DFTPP